
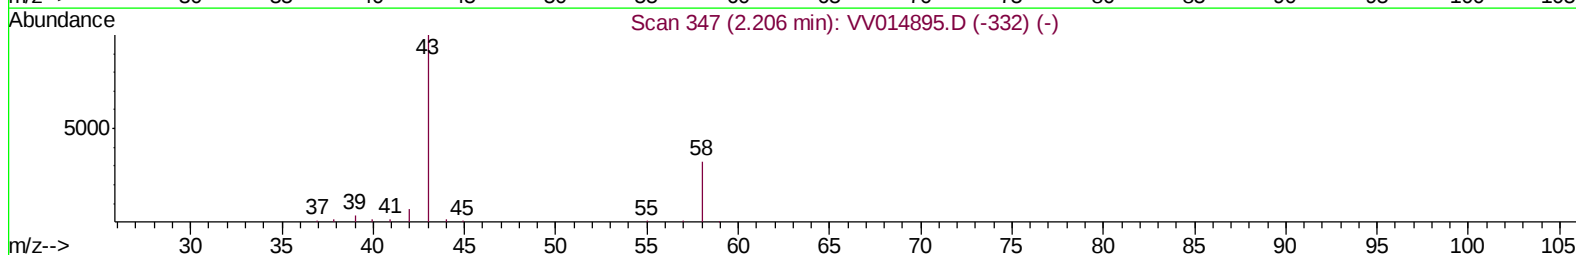
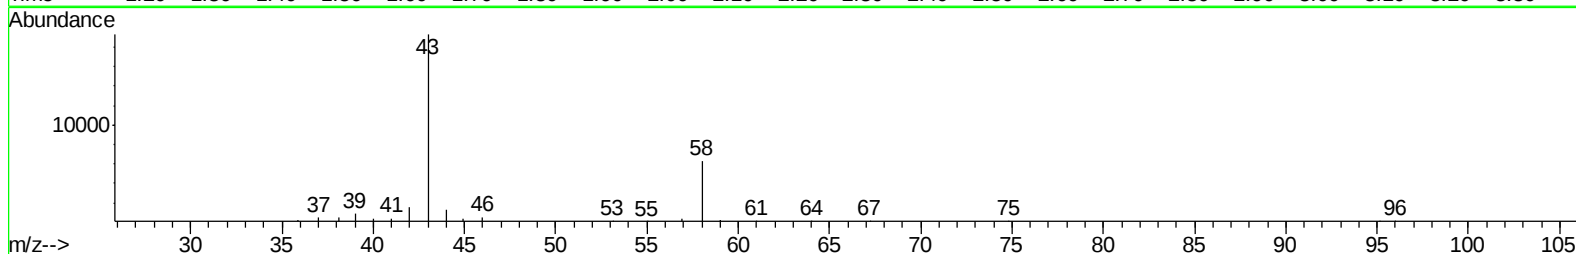


Data File : VV014908.D
Acq On : 13 Mar 2020 16:54
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 13 17:27:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 13 04:10:22 2020
Response via : Initial Calibration

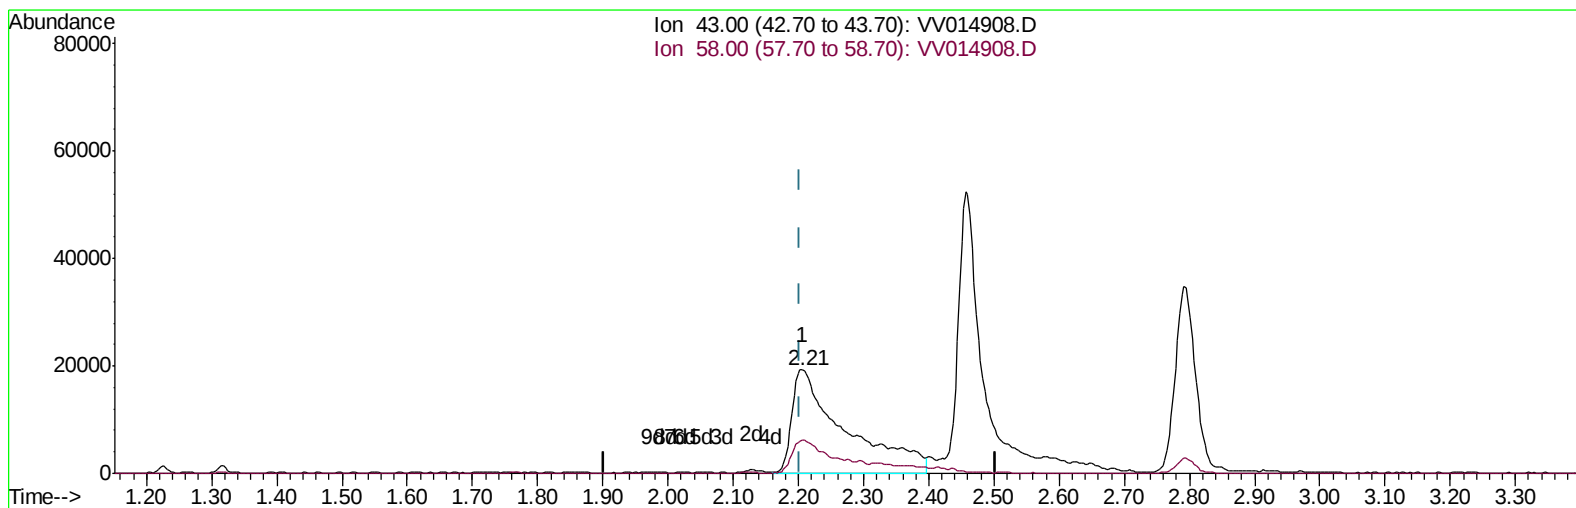

TIC: VV014908.D

(13) Acetone (T)

2.206min (+0.003) 66.71ug/L m

response 109523

Ion	Exp%	Act%
43.00	100	100
58.00	31.10	13.89
0.00	0.00	0.00
0.00	0.00	0.00