
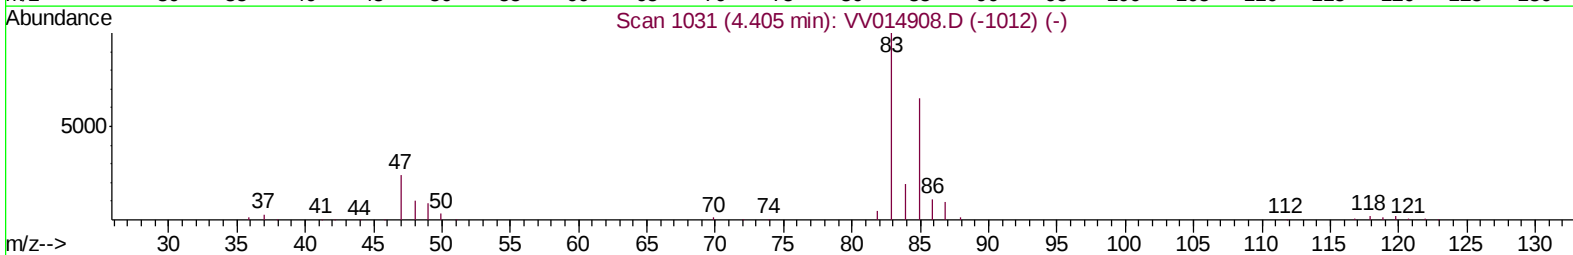
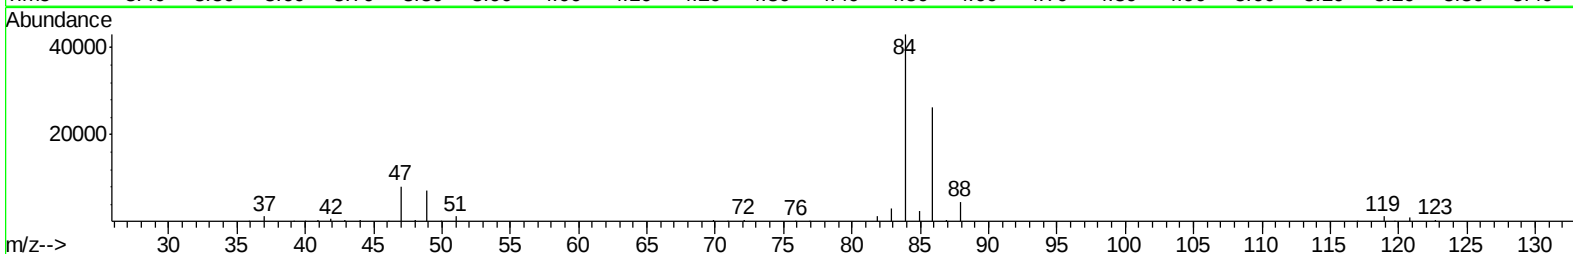


Data File : VV014912.D
Acq On : 13 Mar 2020 18:42
Operator : SY/MD
Sample : L1858-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Mar 16 01:39:13 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 16 01:36:12 2020
Response via : Initial Calibration

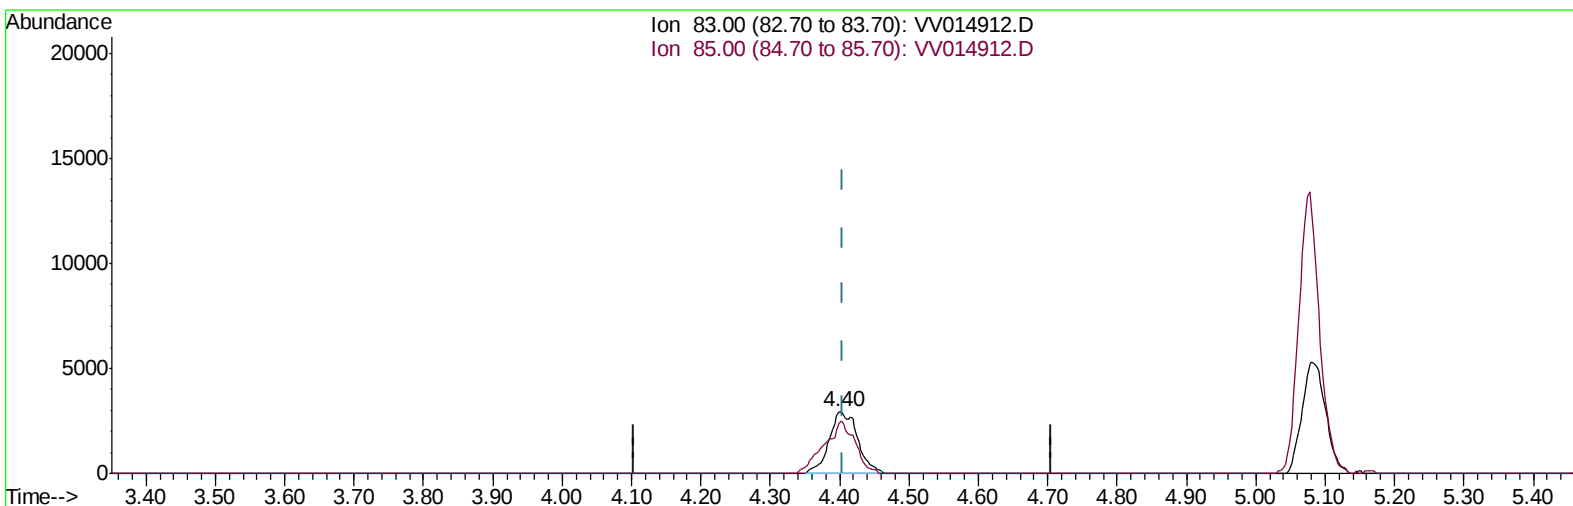

TIC: VV014912.D

(25) Chloroform (T)

4.399min (-0.006) 1.55ug/L m

response 8399

Ion	Exp%	Act%
83.00	100	100
85.00	64.50	81.88
0.00	0.00	0.00
0.00	0.00	0.00