
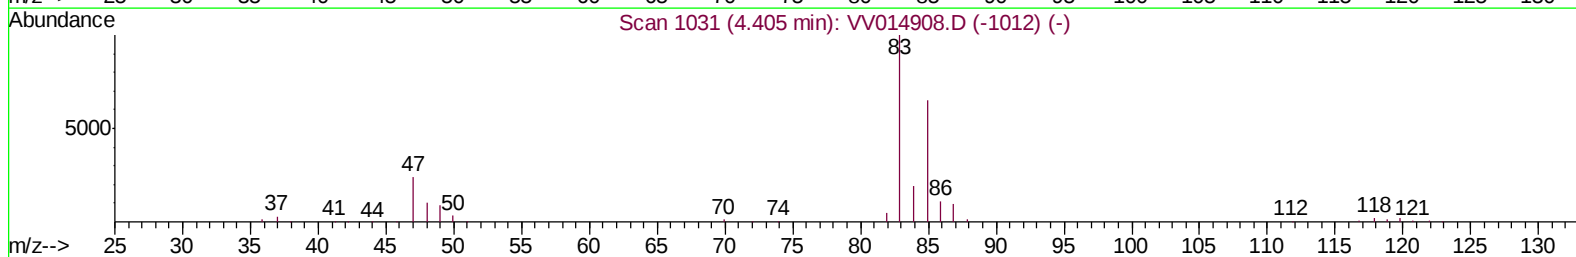
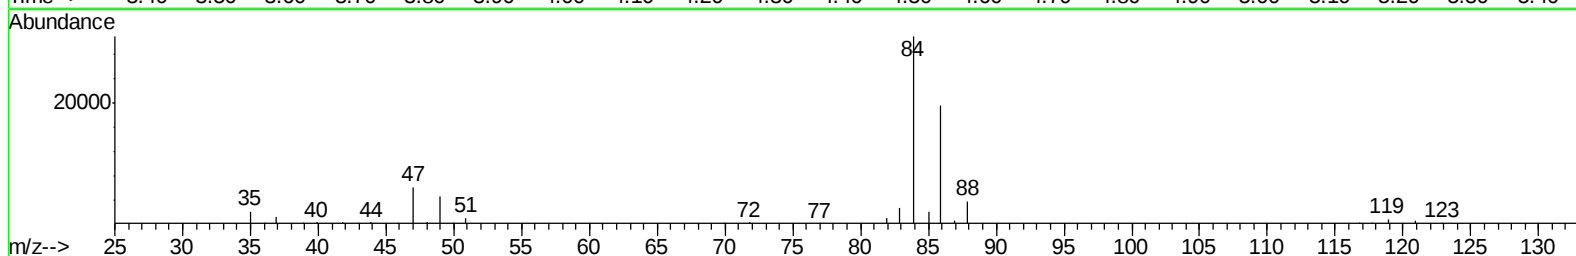


Data File : VV014914.D
Acq On : 13 Mar 2020 19:30
Operator : SY/MD
Sample : L1858-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 16 01:39:33 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 16 01:36:12 2020
Response via : Initial Calibration

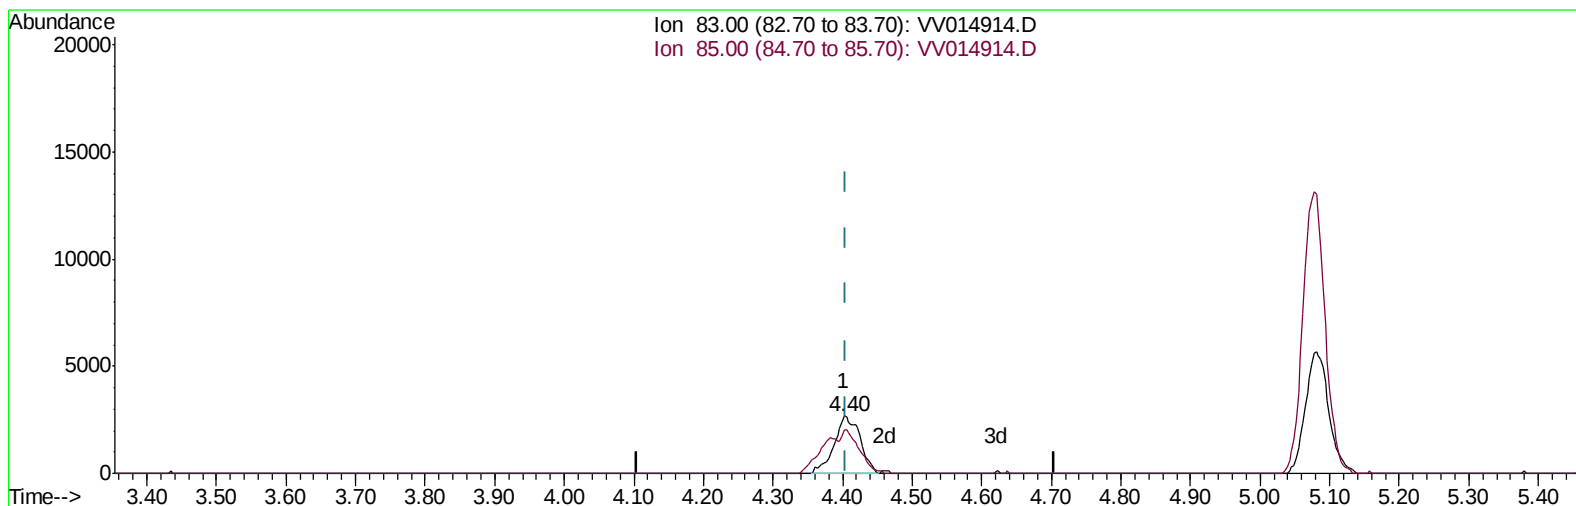

TIC: VV014914.D

(25) Chloroform (T)

4.402min (-0.003) 1.25ug/L m

response 6903

Ion	Exp%	Act%
83.00	100	100
85.00	64.50	75.48
0.00	0.00	0.00
0.00	0.00	0.00