
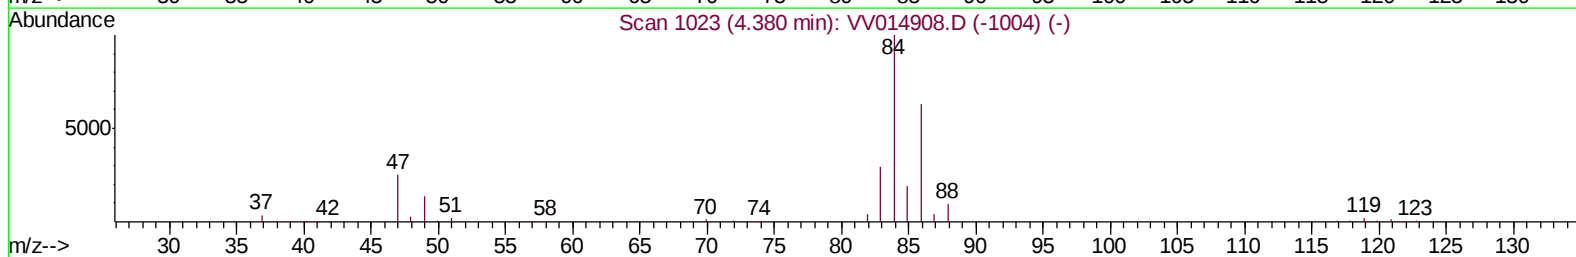
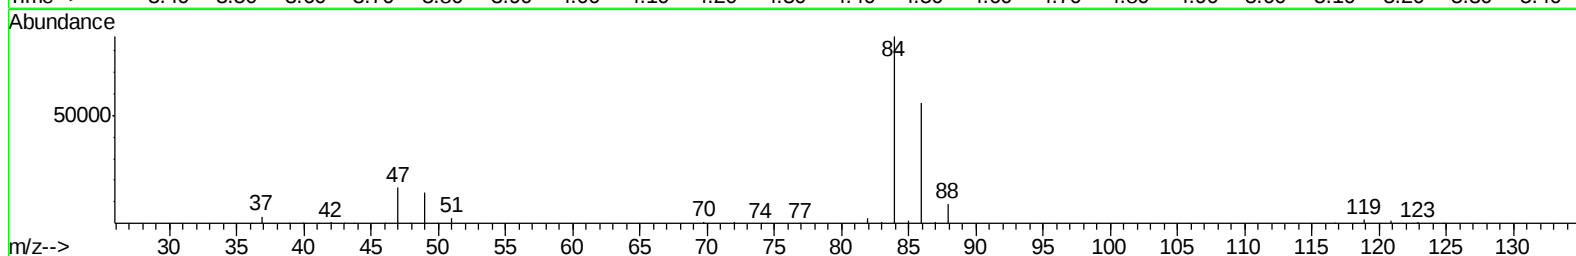


Data File : VV014915.D
Acq On : 13 Mar 2020 19:54
Operator : SY/MD
Sample : L1858-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 16 01:39:42 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 16 01:36:12 2020
Response via : Initial Calibration

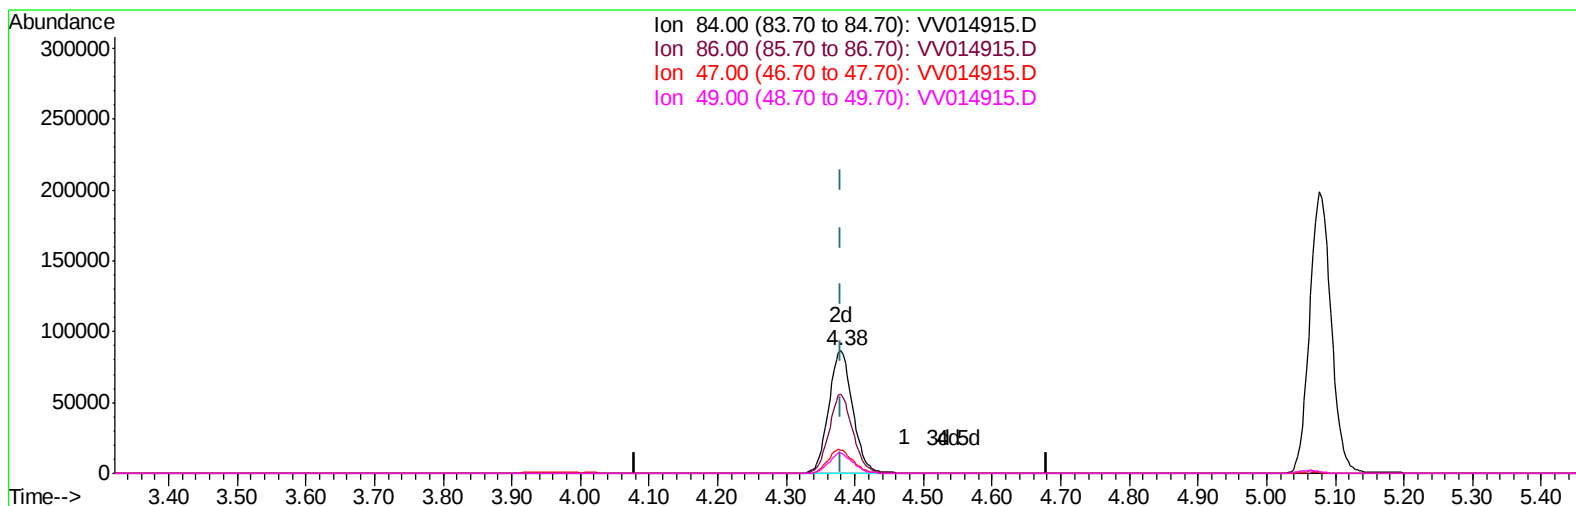

TIC: VV014915.D

(24) Chloroform-d (S)

4.380min (0.000) 41.67ug/L m

response 209765

Ion	Exp%	Act%
84.00	100	100
86.00	62.80	0.07#
47.00	44.00	0.04#
49.00	25.00	0.02#