
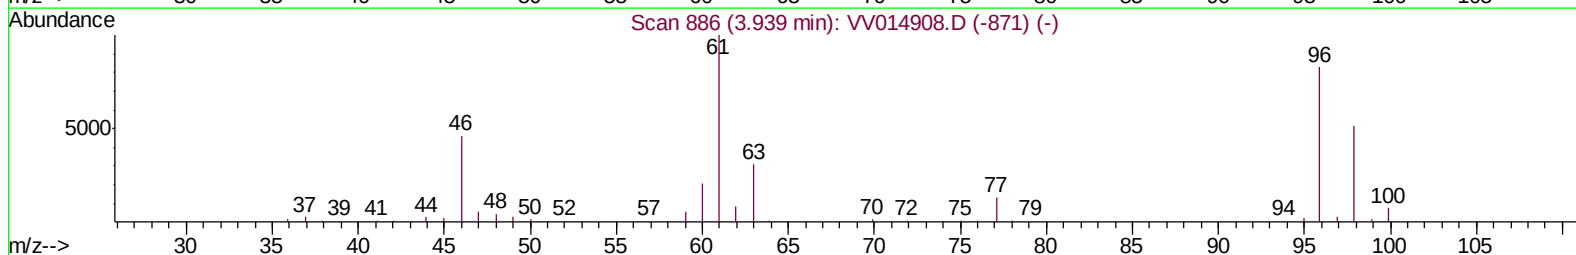
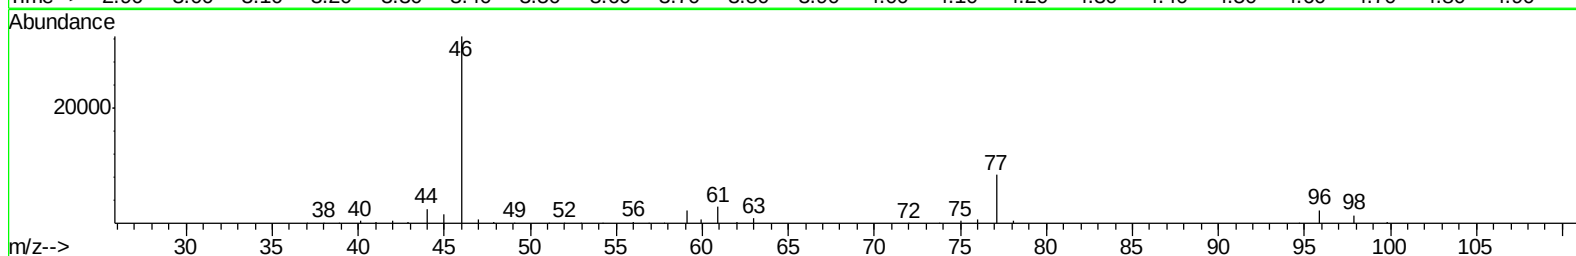


Data File : VV014921.D
Acq On : 13 Mar 2020 22:19
Operator : SY/MD
Sample : L1884-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 16 01:40:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 16 01:36:12 2020
Response via : Initial Calibration

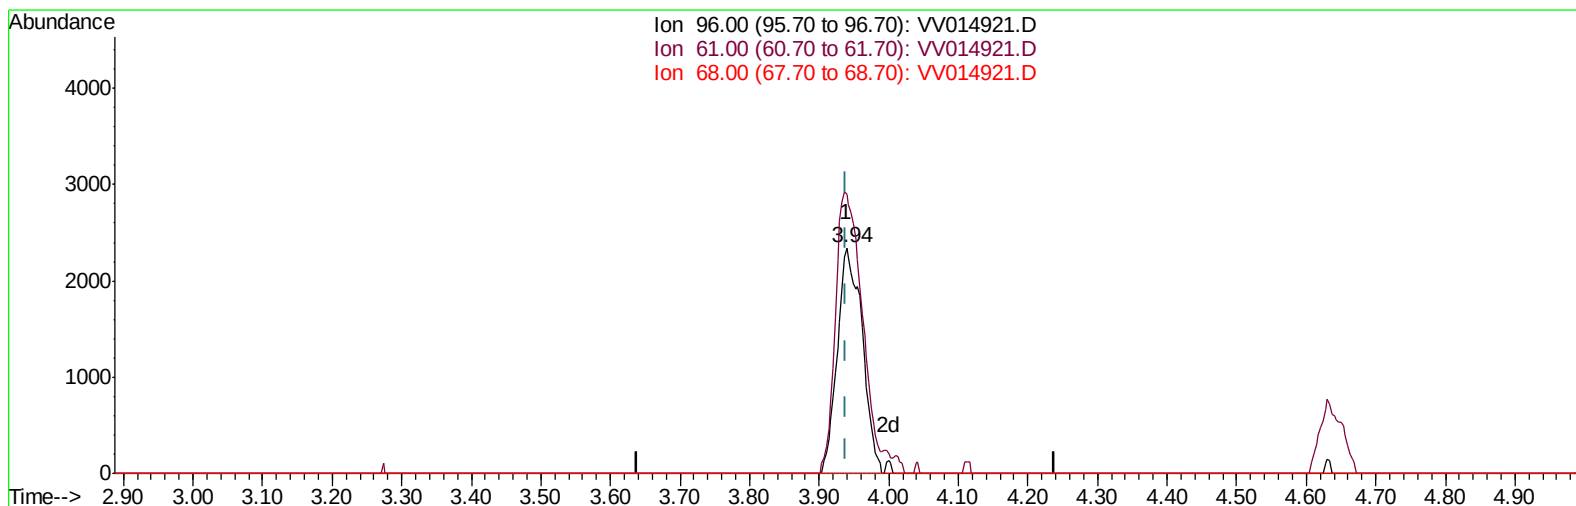

TIC: VV014921.D

(20) cis-1,2-Dichloroethene (T)

3.939min (+0.000) 1.98ug/L m

response 5785

Ion	Exp%	Act%
96.00	100	100
61.00	131.70	123.43
68.00	0.00	0.00
0.00	0.00	0.00