
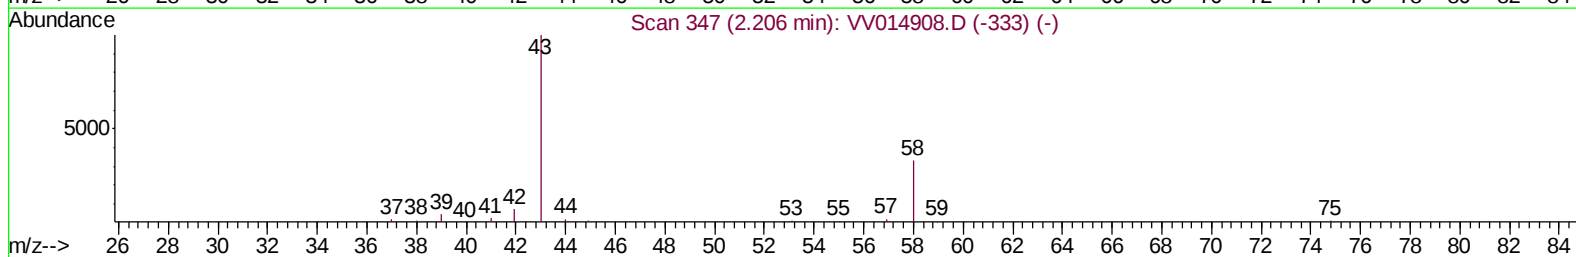
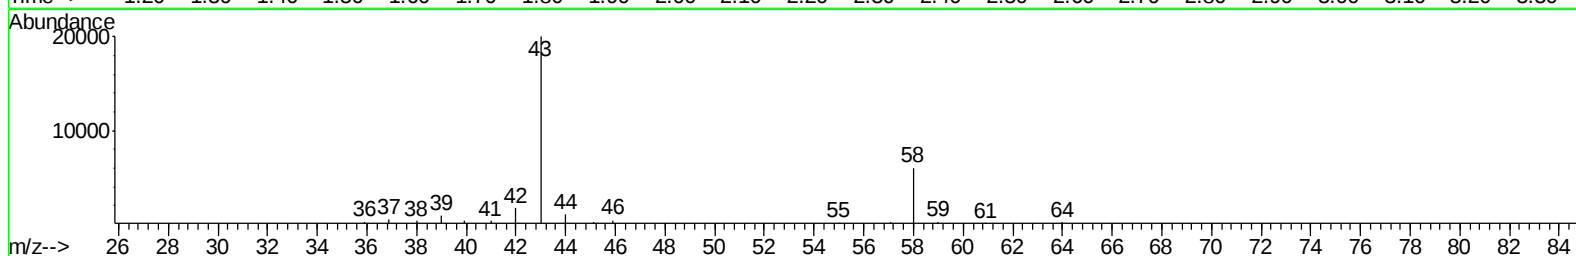


Data File : VV014932.D
Acq On : 14 Mar 2020 02:46
Operator : SY/MD
Sample : VSTDCCC050EC
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Quant Time: Mar 16 01:42:17 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 16 01:36:12 2020
Response via : Initial Calibration

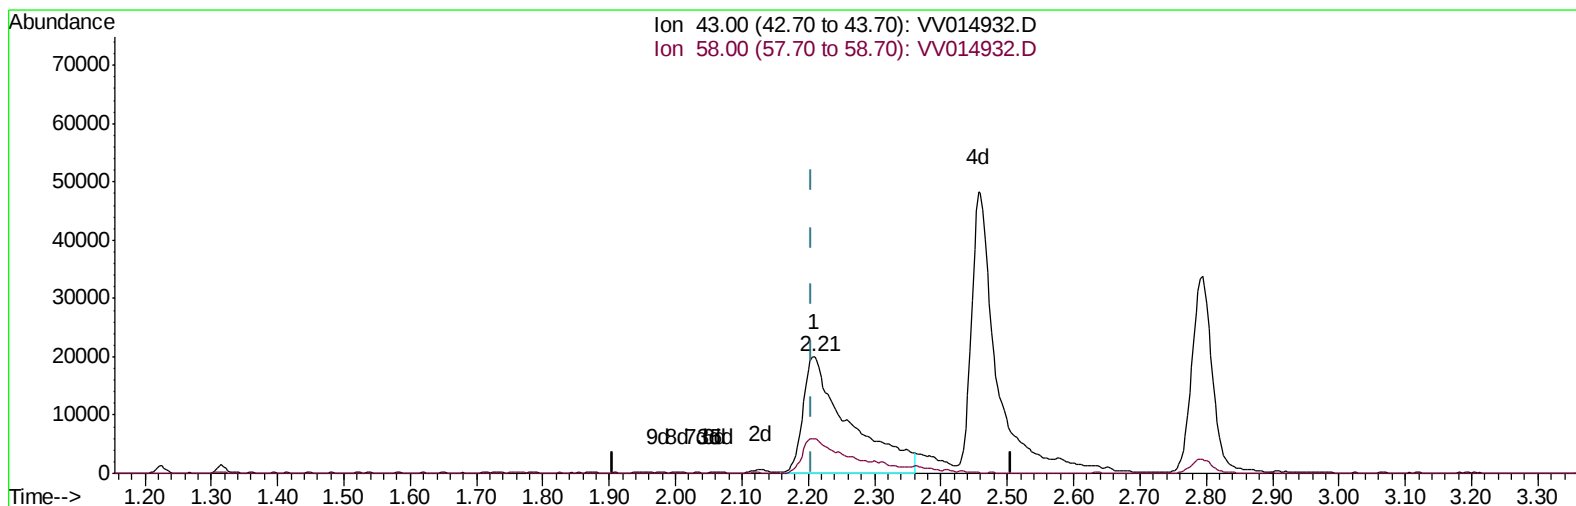

TIC: VV014932.D

(13) Acetone (T)

2.209min (+0.003) 59.67ug/L m

response 96869

Ion	Exp%	Act%
43.00	100	100
58.00	31.10	17.47
0.00	0.00	0.00
0.00	0.00	0.00