

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031320\
 Data File : VV014909.D
 Acq On : 13 Mar 2020 17:23
 Operator : SY/MD
 Sample : VV0313WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	62	69	81	rVB	148996	155803	14.08%	1.869%
2	1.573	144	150	164	rVB	100659	124456	11.24%	1.493%
3	2.116	310	319	337	rVB	233047	332139	30.01%	3.985%
4	2.521	439	445	448	rBV6	1251	1548	0.14%	0.019%
5	2.582	463	464	468	rBV2	444	281	0.03%	0.003%
6	2.888	557	559	561	rBV2	447	238	0.02%	0.003%
7	3.113	627	629	633	rBV3	432	297	0.03%	0.004%
8	3.196	654	655	659	rBV2	422	226	0.02%	0.003%
9	3.229	659	665	667	rBV5	732	720	0.07%	0.009%
10	3.274	677	679	682	rVB2	361	218	0.02%	0.003%
11	3.441	726	731	733	rBV3	465	351	0.03%	0.004%
12	3.518	751	755	759	rVB2	400	348	0.03%	0.004%
13	3.547	759	764	767	rBV4	613	479	0.04%	0.006%
14	3.602	778	781	785	rVB	337	233	0.02%	0.003%
15	3.631	787	790	793	rVB2	372	257	0.02%	0.003%
16	3.865	858	863	865	rBV2	427	352	0.03%	0.004%
17	3.936	873	885	917	rBV	47914	195380	17.65%	2.344%
18	4.746	1133	1137	1138	rBV	493	229	0.02%	0.003%
19	4.817	1155	1159	1161	rBV2	577	431	0.04%	0.005%
20	4.872	1174	1176	1181	rVB	460	234	0.02%	0.003%
21	5.013	1216	1220	1221	rBV3	328	236	0.02%	0.003%
22	5.071	1221	1238	1257	rBV2	451540	1106775	100.00%	13.280%
23	5.415	1342	1345	1348	rBV2	665	428	0.04%	0.005%
24	5.466	1358	1361	1364	rVB3	587	360	0.03%	0.004%
25	5.534	1380	1382	1386	rVB	435	240	0.02%	0.003%
26	5.553	1386	1388	1392	rVB	442	261	0.02%	0.003%
27	5.589	1393	1399	1401	rBV2	375	358	0.03%	0.004%
28	5.640	1401	1415	1437	rBV	352734	699008	63.16%	8.387%
29	5.958	1511	1514	1515	rBV3	424	208	0.02%	0.002%
30	6.019	1529	1533	1534	rBV2	419	268	0.02%	0.003%
31	6.093	1542	1556	1579	rBV	240308	492463	44.50%	5.909%
32	6.328	1627	1629	1633	rBV3	434	239	0.02%	0.003%
33	6.354	1635	1637	1640	rBV	360	246	0.02%	0.003%
34	6.405	1650	1653	1655	rBV2	437	311	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031320\
 Data File : VV014909.D
 Acq On : 13 Mar 2020 17:23
 Operator : SY/MD
 Sample : VV0313WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

35	6.473	1671	1674	1676	rVB	709	330	0.03%	0.004%
36	6.643	1725	1727	1730	rVB2	571	220	0.02%	0.003%
37	6.762	1760	1764	1765	rBV	460	404	0.04%	0.005%
38	6.823	1782	1783	1788	rVB2	307	225	0.02%	0.003%
39	6.910	1808	1810	1813	rVB2	434	220	0.02%	0.003%
40	7.007	1828	1840	1862	rBV	137601	249960	22.58%	2.999%
41	7.161	1885	1888	1892	rVB4	746	591	0.05%	0.007%
42	7.183	1892	1895	1898	rVB2	651	387	0.03%	0.005%
43	7.203	1898	1901	1903	rBV3	474	275	0.02%	0.003%
44	7.228	1907	1909	1912	rVB3	594	246	0.02%	0.003%
45	7.248	1912	1915	1917	rBV	509	356	0.03%	0.004%
46	7.338	1930	1943	1961	rBV	560468	963090	87.02%	11.556%
47	7.643	2027	2038	2056	rBV	94786	167254	15.11%	2.007%
48	7.839	2097	2099	2102	rBV3	436	215	0.02%	0.003%
49	7.884	2109	2113	2115	rBV2	439	285	0.03%	0.003%
50	7.955	2133	2135	2137	rVV	625	344	0.03%	0.004%
51	8.064	2167	2169	2172	rVB2	526	226	0.02%	0.003%
52	8.116	2172	2185	2222	rBV	286677	655358	59.21%	7.863%
53	8.444	2282	2287	2290	rBV3	1241	1283	0.12%	0.015%
54	8.579	2325	2329	2332	rVV3	647	482	0.04%	0.006%
55	8.640	2346	2348	2352	rBV2	356	214	0.02%	0.003%
56	8.756	2382	2384	2388	rBV3	460	359	0.03%	0.004%
57	8.871	2408	2420	2450	rBV	524067	861037	77.80%	10.331%
58	9.199	2519	2522	2527	rBV2	493	493	0.04%	0.006%
59	9.254	2537	2539	2543	rVB2	654	396	0.04%	0.005%
60	9.289	2543	2550	2554	rBV2	583	677	0.06%	0.008%
61	9.351	2564	2569	2571	rBV	350	280	0.03%	0.003%
62	9.396	2580	2583	2585	rVB	495	258	0.02%	0.003%
63	9.415	2586	2589	2591	rBV	518	300	0.03%	0.004%
64	9.550	2628	2631	2632	rBV	396	227	0.02%	0.003%
65	9.662	2663	2666	2668	rBV2	566	343	0.03%	0.004%
66	9.794	2705	2707	2711	rVB2	400	235	0.02%	0.003%
67	9.990	2764	2768	2770	rBV3	434	314	0.03%	0.004%
68	10.068	2788	2792	2796	rBV	483	476	0.04%	0.006%
69	10.238	2832	2845	2860	rBV	353025	571956	51.68%	6.863%
70	10.469	2914	2917	2919	rBV2	530	230	0.02%	0.003%
71	10.486	2919	2922	2923	rBV	435	203	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031320\
 Data File : VV014909.D
 Acq On : 13 Mar 2020 17:23
 Operator : SY/MD
 Sample : VV0313WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis

72	10.534	2933	2937	2940	rBV3	447	479	0.04%	0.006%
73	10.785	3013	3015	3020	rBV	738	363	0.03%	0.004%
74	10.894	3047	3049	3052	rVB2	412	234	0.02%	0.003%
75	10.939	3057	3063	3068	rVB3	1065	1237	0.11%	0.015%
76	11.068	3099	3103	3107	rBV2	582	452	0.04%	0.005%
77	11.145	3124	3127	3131	rVB2	969	699	0.06%	0.008%
78	11.180	3131	3138	3140	rBV2	595	770	0.07%	0.009%
79	11.199	3140	3144	3145	rBV3	959	591	0.05%	0.007%
80	11.270	3154	3166	3184	rBV	551479	846080	76.45%	10.152%
81	11.505	3236	3239	3241	rBV	425	276	0.02%	0.003%
82	11.527	3241	3246	3252	rVV4	538	705	0.06%	0.008%
83	11.595	3264	3267	3270	rBV2	346	210	0.02%	0.003%
84	11.646	3270	3283	3299	rBV	554947	871060	78.70%	10.452%
85	11.791	3324	3328	3329	rBV2	372	237	0.02%	0.003%
86	11.881	3353	3356	3359	rBV2	640	381	0.03%	0.005%
87	11.971	3382	3384	3386	rBV2	496	204	0.02%	0.002%
88	12.042	3402	3406	3407	rBV	403	246	0.02%	0.003%
89	12.100	3422	3424	3428	rBV2	379	238	0.02%	0.003%
90	12.370	3506	3508	3512	rBV3	450	371	0.03%	0.004%
91	12.408	3519	3520	3527	rVB	660	405	0.04%	0.005%
92	12.450	3531	3533	3535	rBV2	685	351	0.03%	0.004%
93	12.666	3595	3600	3610	rVB4	2674	3889	0.35%	0.047%
94	12.707	3610	3613	3614	rBV	537	268	0.02%	0.003%
95	12.984	3697	3699	3702	rVB2	601	301	0.03%	0.004%
96	13.077	3725	3728	3731	rBV2	463	286	0.03%	0.003%
97	13.193	3762	3764	3768	rBV2	420	294	0.03%	0.004%
98	13.524	3859	3867	3879	rBV2	4617	7558	0.68%	0.091%
99	13.939	3993	3996	3998	rBV2	606	338	0.03%	0.004%
100	14.440	4150	4152	4156	rBV3	654	402	0.04%	0.005%


Sum of corrected areas: 8334295

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031320\
Data File : VV014909.D
Acq On : 13 Mar 2020 17:23
Operator : SY/MD
Sample : VV0313WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK85

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

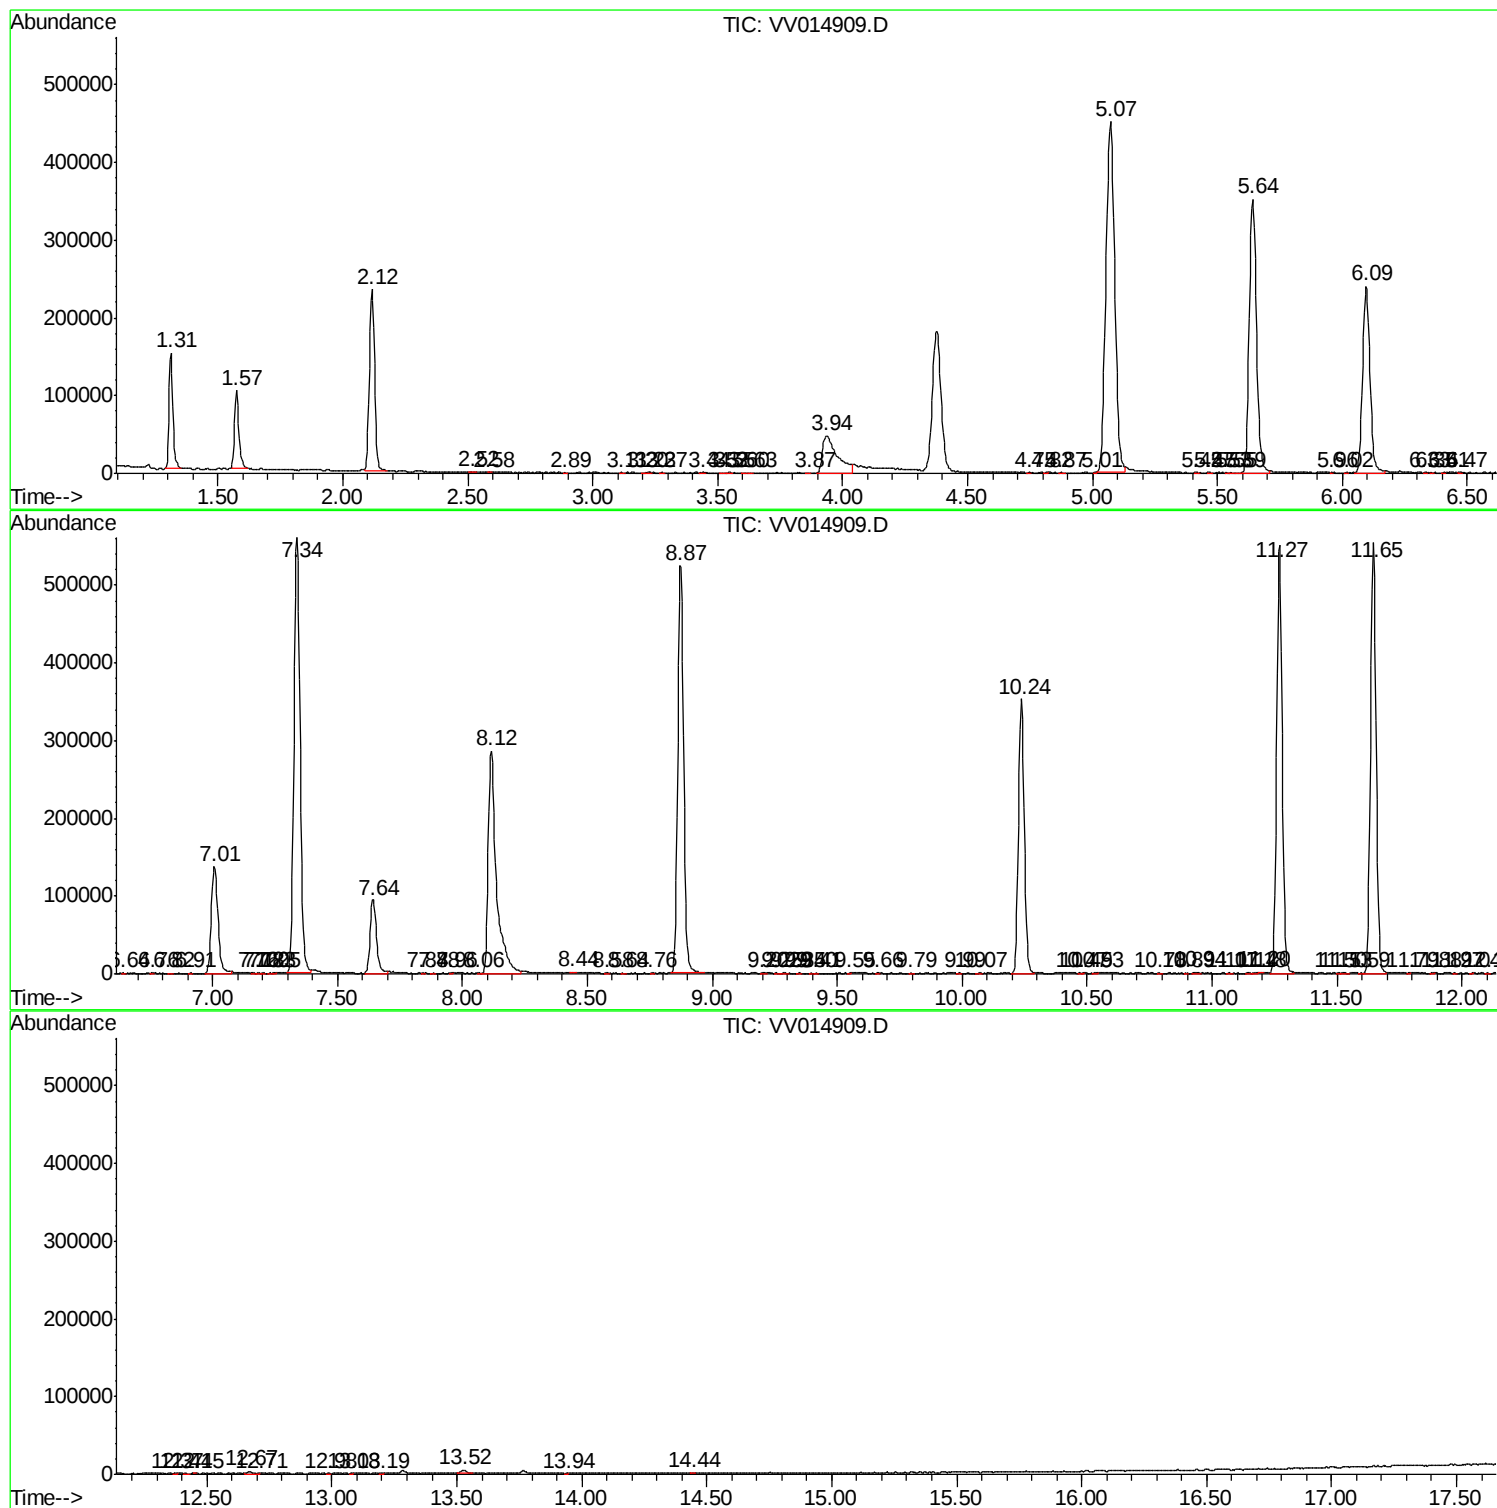

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031320\
Data File : VV014909.D
Acq On : 13 Mar 2020 17:23
Operator : SY/MD
Sample : VV0313WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK85

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031320\
Data File : VV014909.D
Acq On : 13 Mar 2020 17:23
Operator : SY/MD
Sample : VV0313WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK85

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc