


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031320\
 Data File : VV014894.D
 Acq On : 13 Mar 2020 10:05
 Operator : SY/MD
 Sample : BFB63
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 16 01:36:12 2020

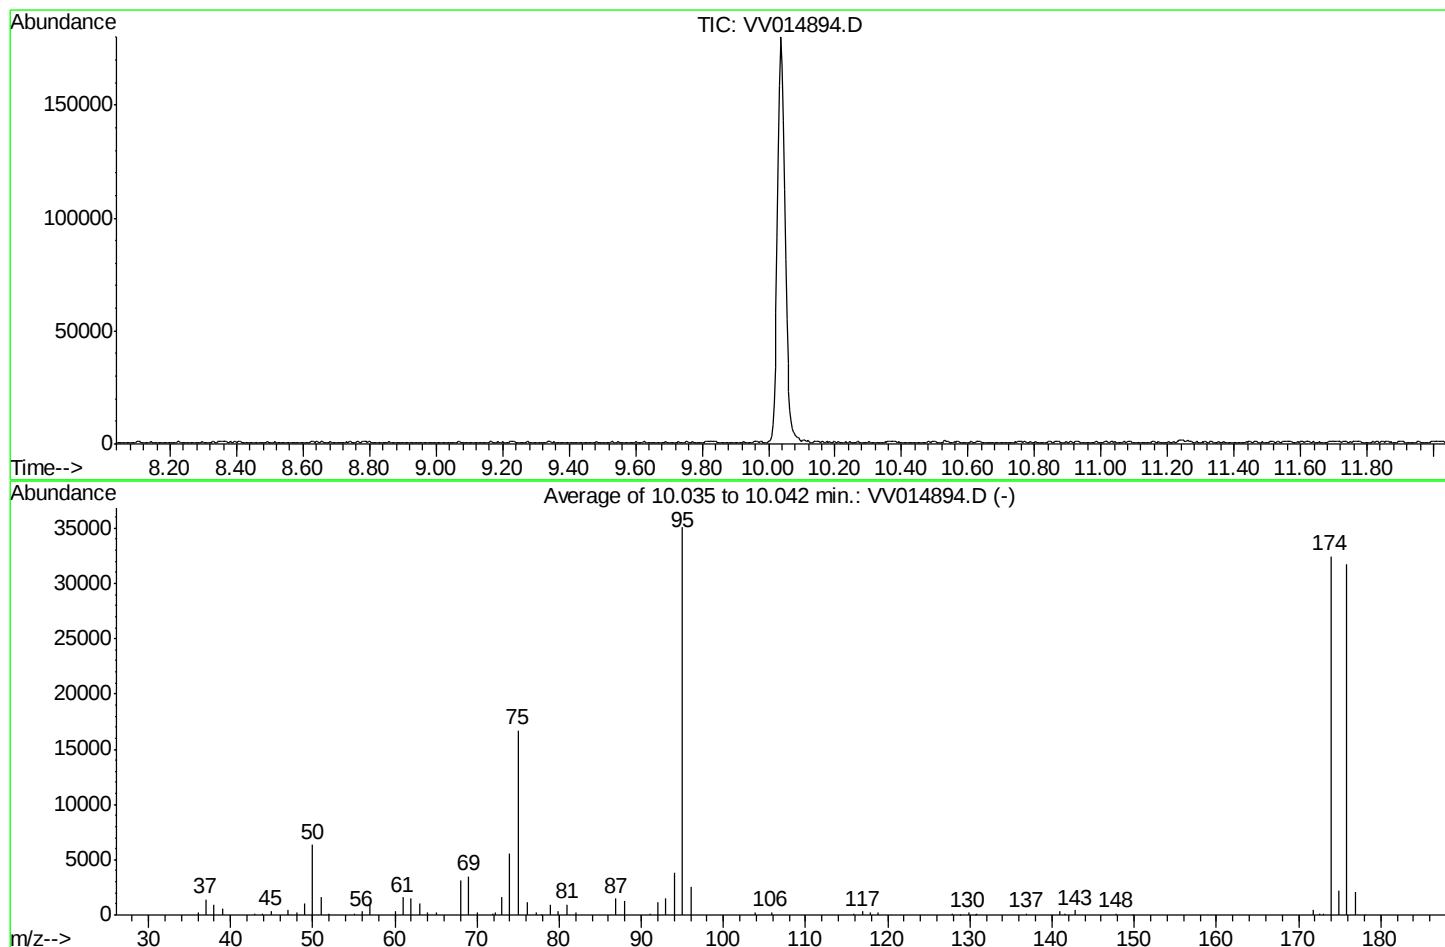

AutoFind: Scans 2782, 2783, 2784; Background Corrected with Scan 2770

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	6335	PASS
75	95	30	80	47.6	16711	PASS
95	95	100	100	100.0	35072	PASS
96	95	5	9	7.3	2565	PASS
173	174	0.00	2	0.5	150	PASS
174	95	50	120	92.5	32440	PASS
175	174	5	9	6.8	2209	PASS
176	174	95	101	97.7	31680	PASS
177	176	5	9	6.7	2133	PASS

m/z	Abundance
36.10	190.0
37.00	1407.0
38.00	1147.0
39.00	538.0
39.90	205.0
42.80	145.0
43.90	481.0
44.90	379.0
47.00	410.0
48.00	238.0
49.00	1060.0
50.00	6282.0
51.10	1696.0
51.90	226.0
55.10	153.0
56.10	346.0
56.90	892.0
60.00	398.0
61.00	1714.0
62.00	1663.0
63.00	1110.0
63.90	209.0
65.00	330.0
68.00	3272.0
69.00	3608.0
70.00	273.0
71.80	145.0
72.20	123.0
73.00	1820.0
74.00	5648.0
75.00	17272.0
76.00	1209.0
77.10	240.0
77.90	176.0
78.90	925.0
79.90	365.0
81.00	959.0
82.00	258.0
86.90	1487.0
87.90	1185.0
91.00	108.0
92.00	1208.0
92.90	1463.0
94.00	3874.0
95.00	35104.0
96.00	2768.0
103.90	244.0
105.80	228.0
115.90	152.0
116.90	278.0
117.90	175.0
118.80	284.0
127.90	139.0
129.80	231.0
130.60	128.0
136.90	142.0
141.00	462.0
141.60	155.0
142.90	462.0
147.80	184.0
149.80	138.0
171.90	414.0
173.90	31920.0
174.90	2250.0
175.90	32152.0
176.90	2043.0
178.00	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.10	251.0
37.00	1459.0
38.00	987.0
39.00	580.0
39.90	261.0
42.80	115.0
43.90	453.0
45.00	411.0
46.90	502.0
48.00	246.0
49.10	1067.0
50.00	6537.0
51.00	1706.0
52.00	191.0
55.10	135.0
56.00	332.0
57.00	1019.0
60.00	344.0
61.00	1679.0
62.00	1517.0
63.00	1060.0
64.00	262.0
65.00	280.0
68.00	3084.0
69.00	3662.0
70.00	217.0
71.90	179.0
72.10	189.0
73.00	1663.0
74.00	5653.0
75.00	17152.0
76.10	1118.0
77.20	231.0
78.90	906.0
79.80	362.0
81.00	994.0
82.00	311.0
86.90	1554.0
87.90	1353.0
91.00	104.0
92.00	1167.0
92.90	1524.0
94.00	3921.0
95.00	36128.0
96.00	2591.0
103.90	214.0
105.80	274.0
115.90	154.0
116.90	322.0
117.90	194.0
118.80	265.0
127.80	138.0
128.80	100.0
129.80	213.0
130.80	104.0
136.90	153.0
141.00	386.0
141.60	128.0
142.80	471.0
147.80	150.0
171.80	451.0
172.60	201.0
173.10	245.0
173.90	33496.0
174.90	2263.0
175.90	32576.0
176.90	2226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.10	295.0
37.00	1350.0
38.00	805.0
39.00	543.0
39.90	293.0
42.90	122.0
43.90	491.0
45.00	391.0
46.90	507.0
48.00	207.0
49.10	1031.0
50.00	6187.0
51.00	1580.0
52.00	116.0
55.90	353.0
57.00	974.0
60.00	255.0
61.00	1404.0
62.00	1431.0
63.00	1075.0
64.00	294.0
65.00	250.0
68.00	2868.0
69.00	3264.0
70.00	207.0
72.10	232.0
73.00	1299.0
74.00	5242.0
75.00	15709.0
76.00	1096.0
77.10	189.0
79.00	871.0
79.80	345.0
81.00	920.0
82.00	279.0
86.90	1465.0
87.90	1369.0
92.00	1105.0
92.90	1418.0
94.00	3599.0
95.00	33984.0
96.00	2337.0
103.90	161.0
105.80	244.0
115.90	136.0
117.00	320.0
117.90	189.0
118.80	237.0
127.80	142.0
129.90	166.0
130.90	122.0
136.90	154.0
140.90	305.0
142.80	451.0
147.80	117.0
171.80	419.0
172.90	206.0
173.90	31904.0
174.90	2114.0
175.90	30312.0
176.90	2131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Scan 2770 (9.997 min): VV014894.D
BFB63

m/z	Abundance
40.00	384.0
44.00	330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63