

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
Data File : VV020575.D
Acq On : 12 Mar 2021 20:34
Operator : SY/MD
Sample : M1630-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
3/15/2021 10:06:35 AM

Quant Time: Mar 13 02:35:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 13 02:32:38 2021
Response via : Initial Calibration

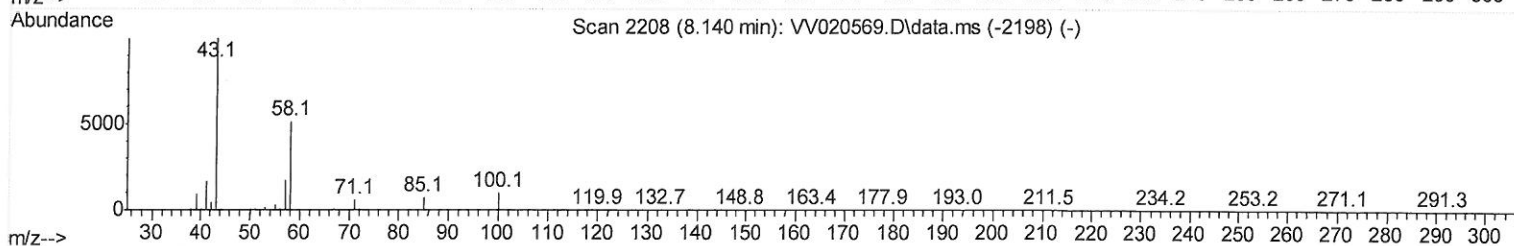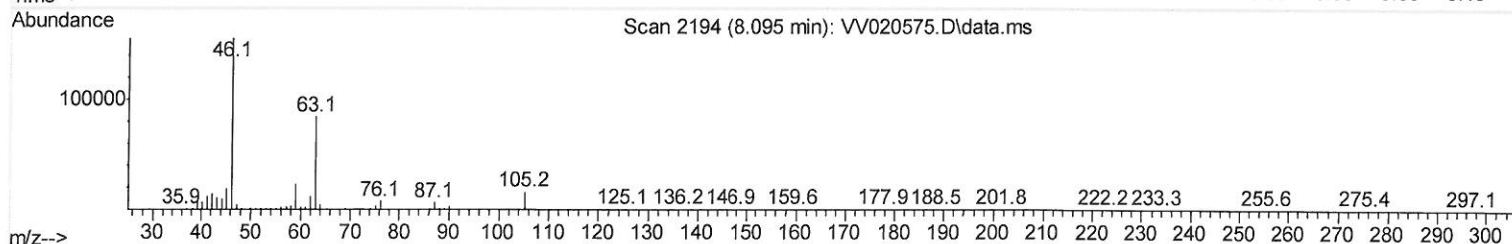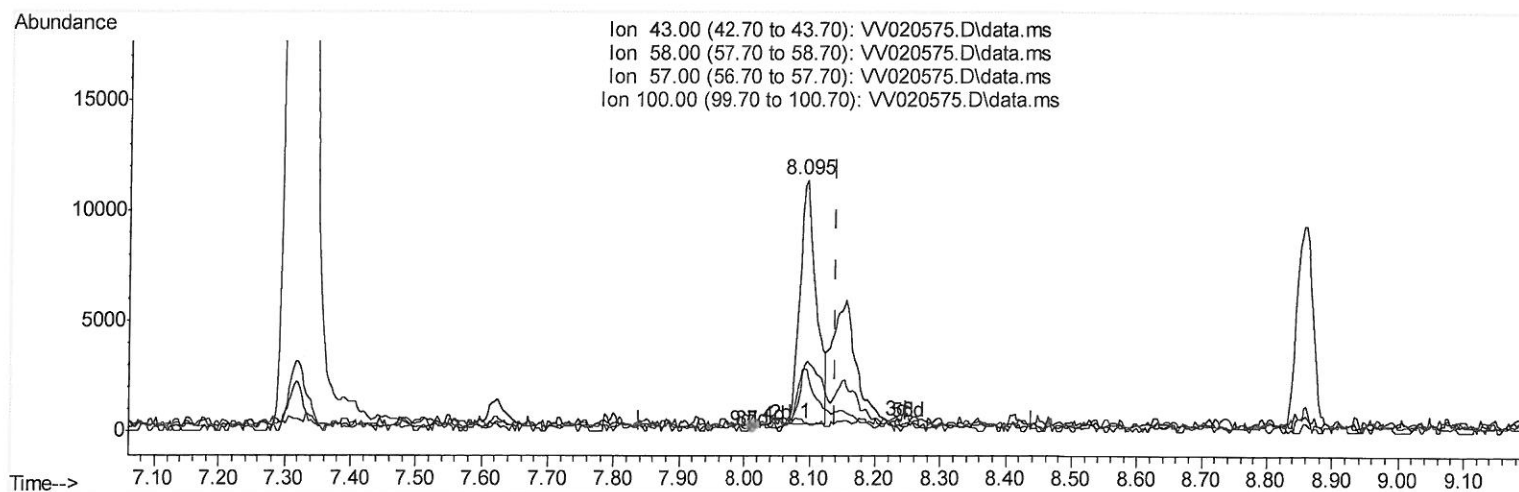

TIC: VV020575.D\data.ms

(48) 2-Hexanone (T)

8.095min (-0.045) 4.51 ug/L

response 19306

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	52.20	31.46#
57.00	18.70	27.04#
100.00	11.10	2.69#

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
Data File : VV020575.D
Acq On : 12 Mar 2021 20:34
Operator : SY/MD
Sample : M1630-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
3/15/2021 10:06:35 AM

Quant Time: Mar 13 02:35:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 13 02:32:38 2021
Response via : Initial Calibration

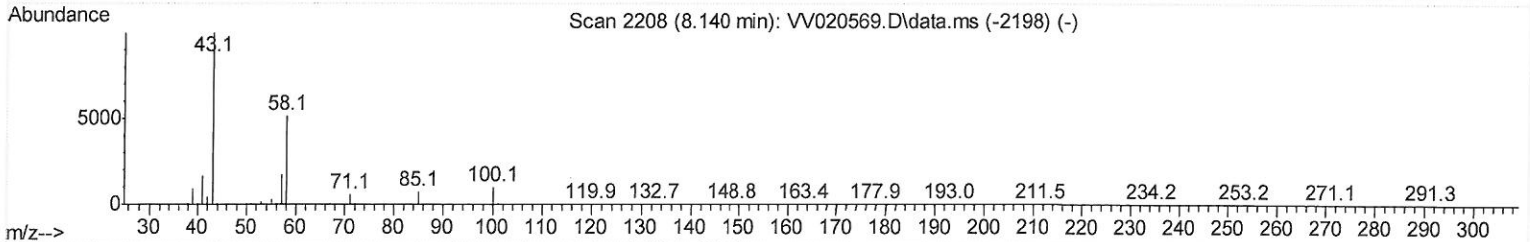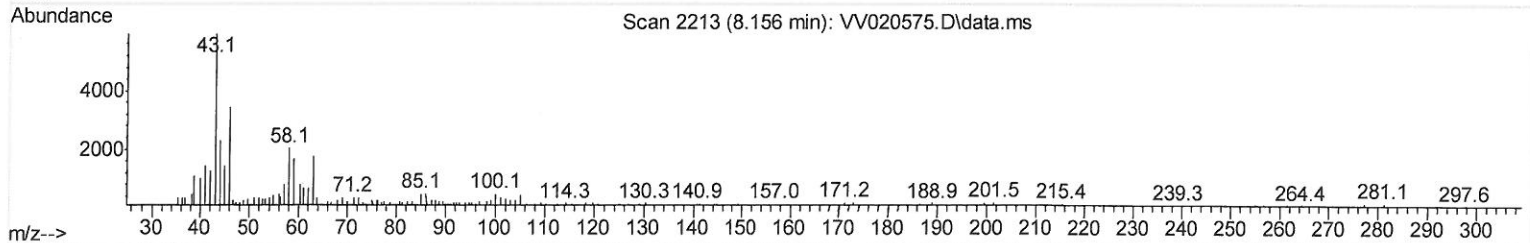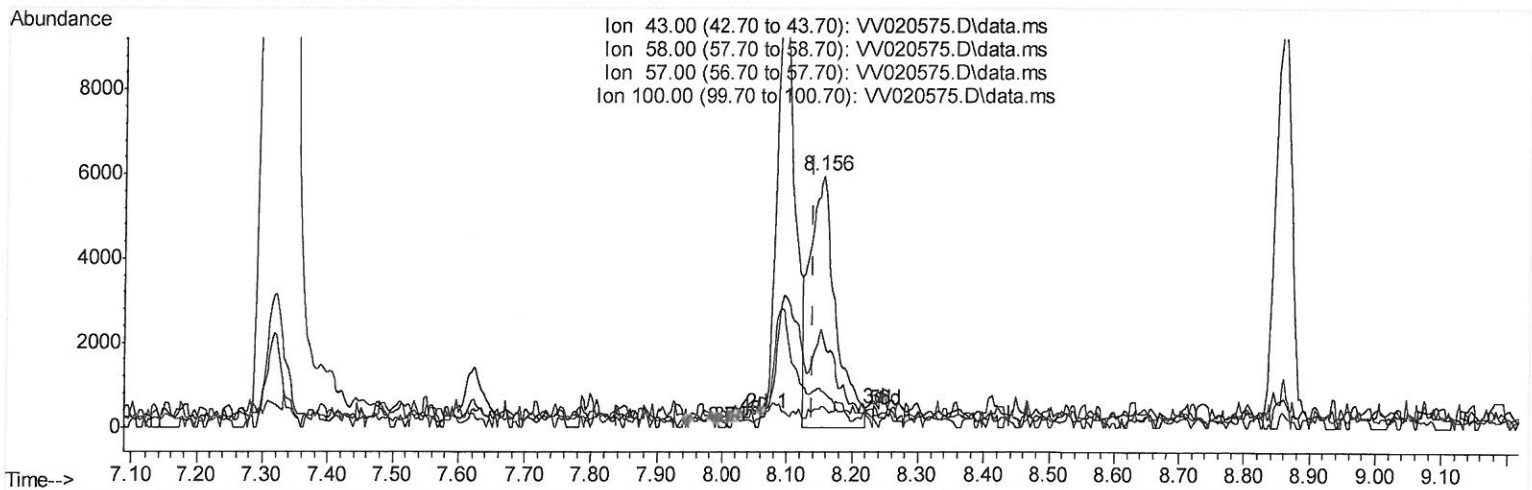

TIC: VV020575.D\data.ms

(48) 2-Hexanone (T)

8.156min (+ 0.016) 3.82 ug/L m

203/17/21 824

response 16353

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	52.20	37.14#
57.00	18.70	31.92#
100.00	11.10	3.17#

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
Data File : VV020575.D
Acq On : 12 Mar 2021 20:34
Operator : SY/MD
Sample : M1630-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
3/15/2021 10:06:35 AM

Quant Time: Mar 13 02:35:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 13 02:32:38 2021
Response via : Initial Calibration

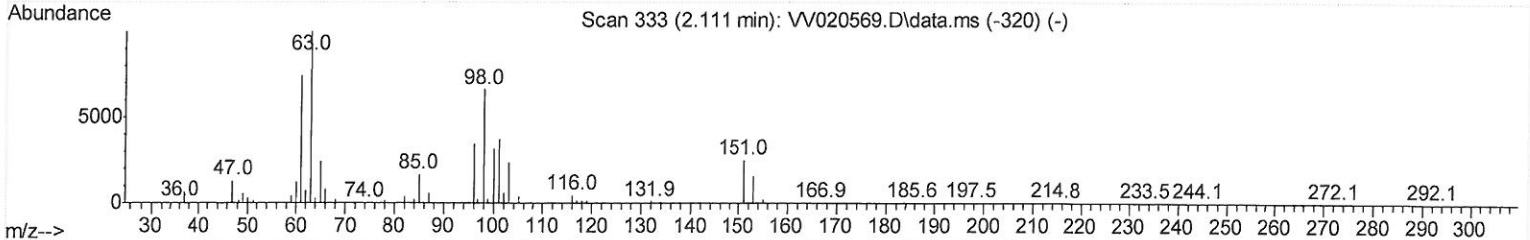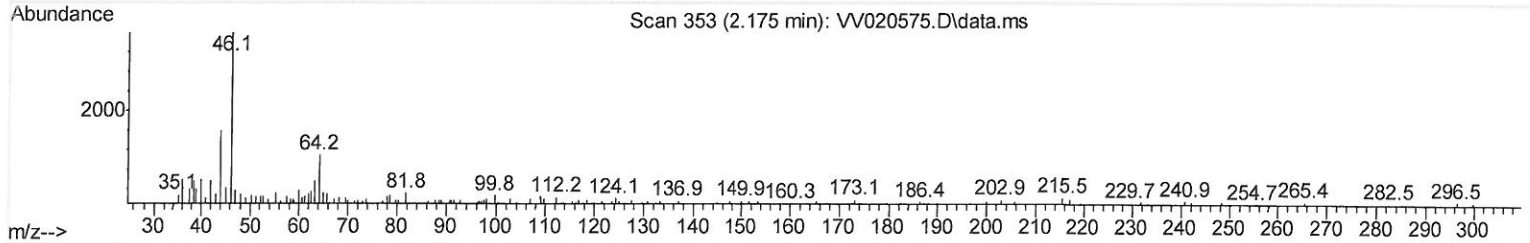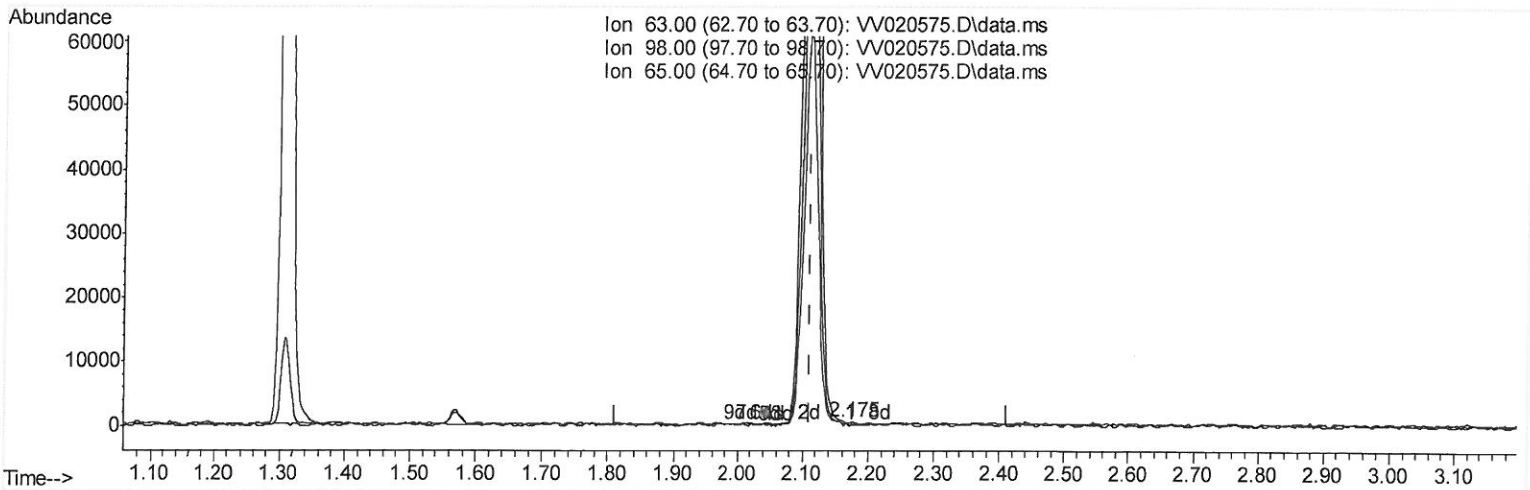

TIC: VV020575.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.175min (+ 0.064) 0.06 ug/L

response 415

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.80	85.54
65.00	23.90	19.04
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
Data File : VV020575.D
Acq On : 12 Mar 2021 20:34
Operator : SY/MD
Sample : M1630-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
3/15/2021 10:06:35 AM

Quant Time: Mar 13 02:35:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 13 02:32:38 2021
Response via : Initial Calibration

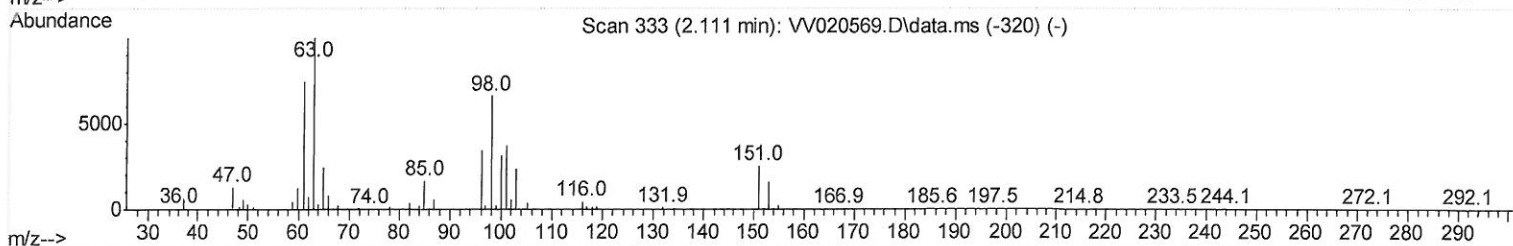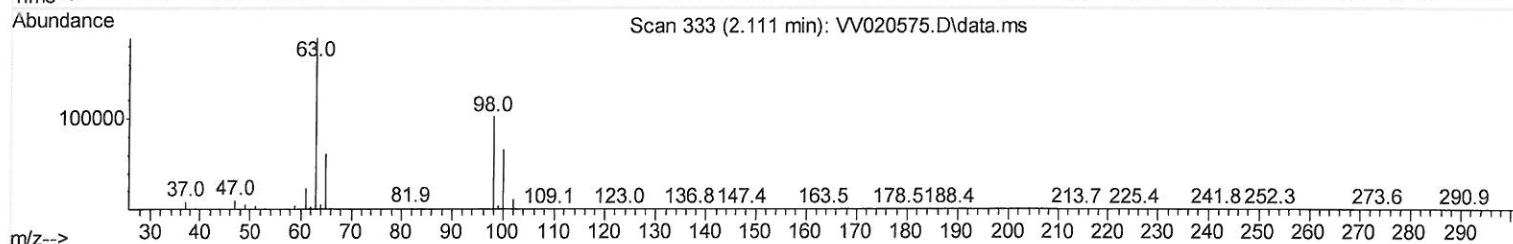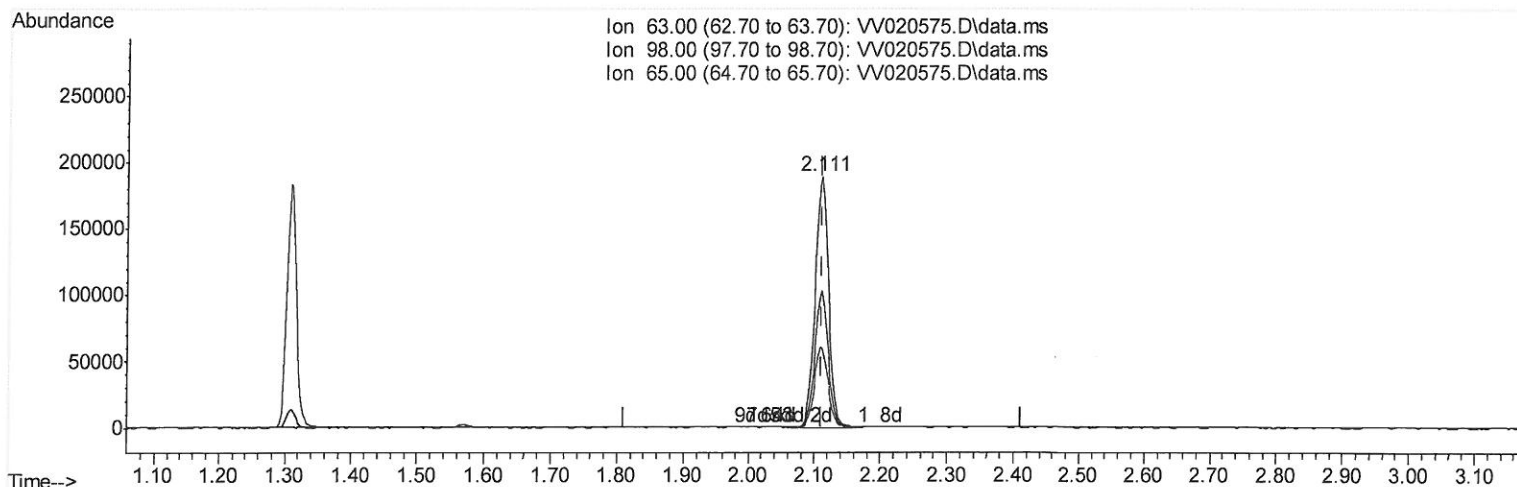

TIC: VV020575.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.111min (-0.000) 37.64 ug/L m

response 272161

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.80	0.13#
65.00	23.90	0.03#
0.00	0.00	0.00

203/17/21 sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031321\
 Data File : VW020575.D
 Acq On : 12 Mar 2021 20:34
 Operator : SY/MD
 Sample : M1630-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Manual Integrations
 APPROVED

MMDadoda
 3/15/2021 10:06:35 AM

Quant Time: Mar 13 02:35:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 13 02:32:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	471530	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	462395	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	201321	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	186709	49.09	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	98.18%		
7) Chloroethane-d5	1.571	69	157005	51.60	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	103.20%		
11) 1,1-Dichloroethene-d2	2.111	63	272161m	37.64	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.28%		
21) 2-Butanone-d5	3.896	46	247382	101.34	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.34%		
24) Chloroform-d	4.352	84	319779	48.37	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.74%		
26) 1,2-Dichloroethane-d4	5.037	65	225825	51.77	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.54%		
32) Benzene-d6	5.053	84	654098	51.20	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.40%		
36) 1,2-Dichloropropane-d6	6.072	67	213516	52.24	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	104.48%		
41) Toluene-d8	7.320	98	569894	50.19	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.38%		
43) trans-1,3-Dichloroprop...	7.625	79	90800	47.53	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.06%		
47) 2-Hexanone-d5	8.091	63	141157	92.30	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.30%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	242281	47.43	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.86%		
64) 1,2-Dichlorobenzene-d4	11.632	152	206277	52.88	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.76%		
Target Compounds						Qvalue
25) Chloroform	4.378	83	11277	1.66	ug/L	93
48) 2-Hexanone	8.156	43	16353m	3.82	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
Data File : VV020575.D
Acq On : 12 Mar 2021 20:34
Operator : SY/MD
Sample : M1630-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
3/15/2021 10:06:35 AM

Quant Time: Mar 13 02:35:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 13 02:32:38 2021
Response via : Initial Calibration

