

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
 Data File : VV020573.D
 Acq On : 12 Mar 2021 19:47
 Operator : SY/MD
 Sample : M1630-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG508

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

Signal : TIC: VV020573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	98	rVB	302411	318788	15.54%	2.106%
2	1.571	158	165	174	rBV	259548	277148	13.51%	1.831%
3	2.111	324	333	351	rVB	507867	748902	36.50%	4.947%
4	2.625	490	493	495	rBV4	4010	2221	0.11%	0.015%
5	2.658	501	503	507	rBV5	4382	2968	0.14%	0.020%
6	2.841	554	560	563	rBV7	4793	5710	0.28%	0.038%
7	2.921	582	585	587	rBV4	2744	2302	0.11%	0.015%
8	3.056	624	627	631	rVB6	5408	4486	0.22%	0.030%
9	3.079	631	634	637	rBV5	3336	2722	0.13%	0.018%
10	3.240	682	684	688	rVB5	5849	4469	0.22%	0.030%
11	3.262	688	691	692	rBV3	4678	2114	0.10%	0.014%
12	3.362	720	722	725	rVB4	4284	2438	0.12%	0.016%
13	3.381	725	728	731	rBV5	3994	2528	0.12%	0.017%
14	3.523	770	772	775	rBV4	4409	2836	0.14%	0.019%
15	3.558	780	783	786	rBV5	3935	3491	0.17%	0.023%
16	3.751	839	843	847	rBV6	4540	3975	0.19%	0.026%
17									

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
 Data File : VV020573.D
 Acq On : 12 Mar 2021 19:47
 Operator : SY/MD
 Sample : M1630-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG508

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Title : VOC Analysis

37	7.580	2031	2034	2038	rBV6	4268	3622	0.18%	0.024%
38	7.625	2038	2048	2064	rVV	173653	299244	14.58%	1.977%
39	8.091	2184	2193	2225	rBV2	442334	886876	43.22%	5.858%
40	8.481	2311	2314	2319	rBV6	2659	3121	0.15%	0.021%
41	8.587	2342	2347	2349	rBV5	3930	3828	0.19%	0.025%
42	8.667	2370	2372	2376	rBV5	3297	2452	0.12%	0.016%
43	8.857	2420	2431	2449	rBV	923126	1467611	71.53%	9.694%
44	9.014	2476	2480	2482	rBV5	3831	2904	0.14%	0.019%
45	9.461	2613	2619	2621	rBV6	4192	4050	0.20%	0.027%
46	9.522	2636	2638	2642	rVB5	3030	2152	0.10%	0.014%
47	9.927	2761	2764	2767	rBV5	4210	2791	0.14%	0.018%
48	10.101	2814	2818	2820	rBV4	4831	2973	0.14%	0.020%
49	10.220	2842	2855	2869	rBV	494722	777784	37.91%	5.137%
50	10.291	2875	2877	2882	rBV6	4683	3229	0.16%	0.021%
51	10.435	2917	2922	2926	rVB8	4277	3773	0.18%	0.025%
52	10.461	2926	2930	2933	rBV6	4877	3389	0.17%	0.022%
53	10.831	3043	3045	3048	rBV4	3288	2292	0.11%	0.015%
54	10.866	3054	3056						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
 Data File : VV020573.D
 Acq On : 12 Mar 2021 19:47
 Operator : SY/MD
 Sample : M1630-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG508

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis


77	13.631	3912	3916	3917	rBV4	3388	2286	0.11%	0.015%
78	13.808	3967	3971	3973	rBV4	5417	4076	0.20%	0.027%
79	13.821	3973	3975	3979	rVV5	3248	2297	0.11%	0.015%
80	13.969	4016	4021	4024	rBV7	5682	5410	0.26%	0.036%
81	14.111	4062	4065	4068	rBV5	3770	2247	0.11%	0.015%
82	14.239	4101	4105	4108	rBV5	2551	2237	0.11%	0.015%
83	14.551	4200	4202	4206	rVB5	5275	3246	0.16%	0.021%
84	14.583	4209	4212	4213	rBV3	4249	2180	0.11%	0.014%
85	14.631	4222	4227	4232	rBV9	4479	5543	0.27%	0.037%
86	14.786	4271	4275	4279	rBV6	4598	4873	0.24%	0.032%
87	14.972	4329	4333	4339	rBV8	4993	4686	0.23%	0.031%
88	15.001	4339	4342	4345	rVB5	3742	2340	0.11%	0.015%
89	15.085	4364	4368	4370	rBV5	3567	2515	0.12%	0.017%
90	15.413	4466	4470	4474	rBV7	4254	4427	0.22%	0.029%
91	15.451	4479	4482	4484	rBV4	3426	2207	0.11%	0.015%
92	15.493	4491	4495	4500					

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
Data File : VV020573.D
Acq On : 12 Mar 2021 19:47
Operator : SY/MD
Sample : M1630-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG508

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

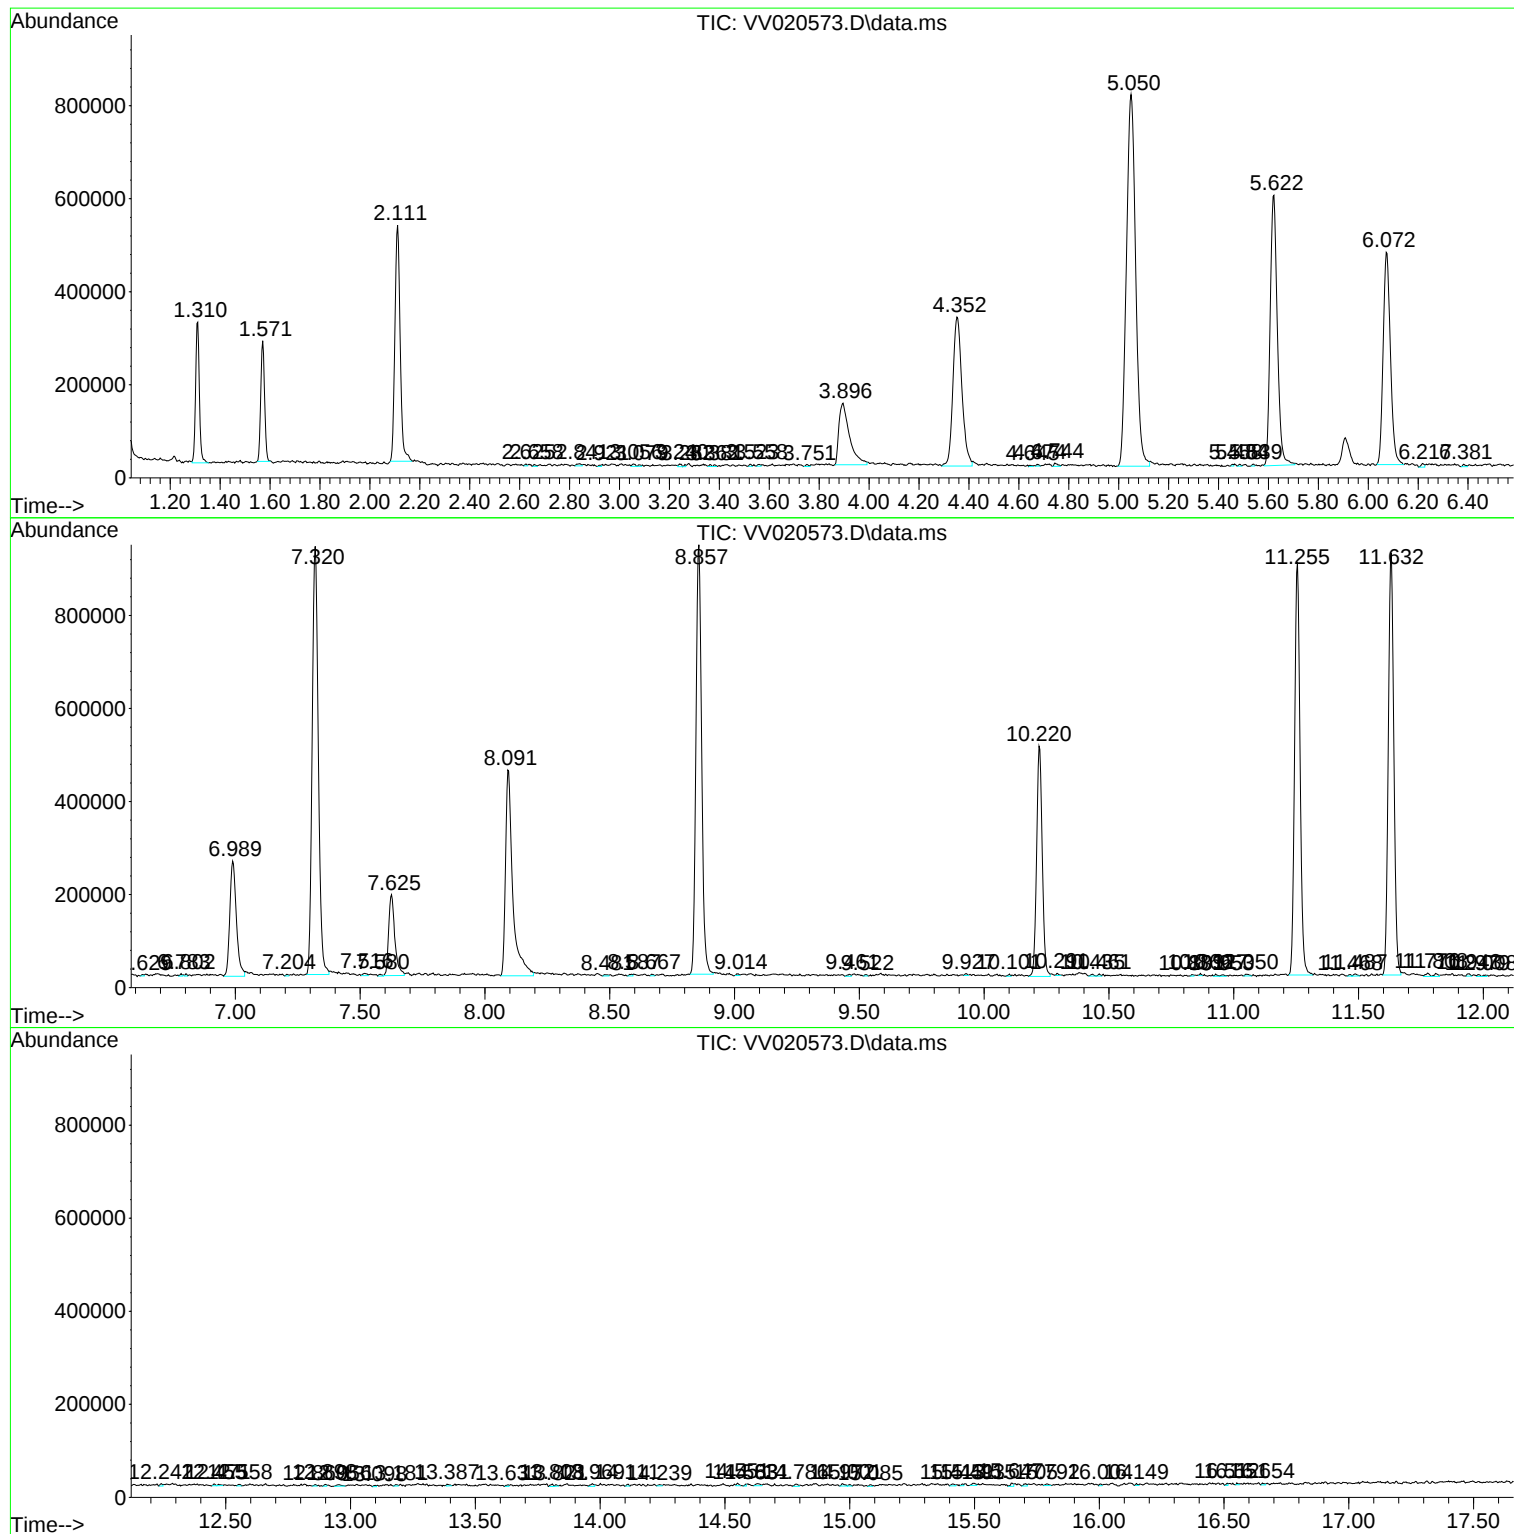

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
Data File : VV020573.D
Acq On : 12 Mar 2021 19:47
Operator : SY/MD
Sample : M1630-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG508

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
Data File : VV020573.D
Acq On : 12 Mar 2021 19:47
Operator : SY/MD
Sample : M1630-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG508

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
