
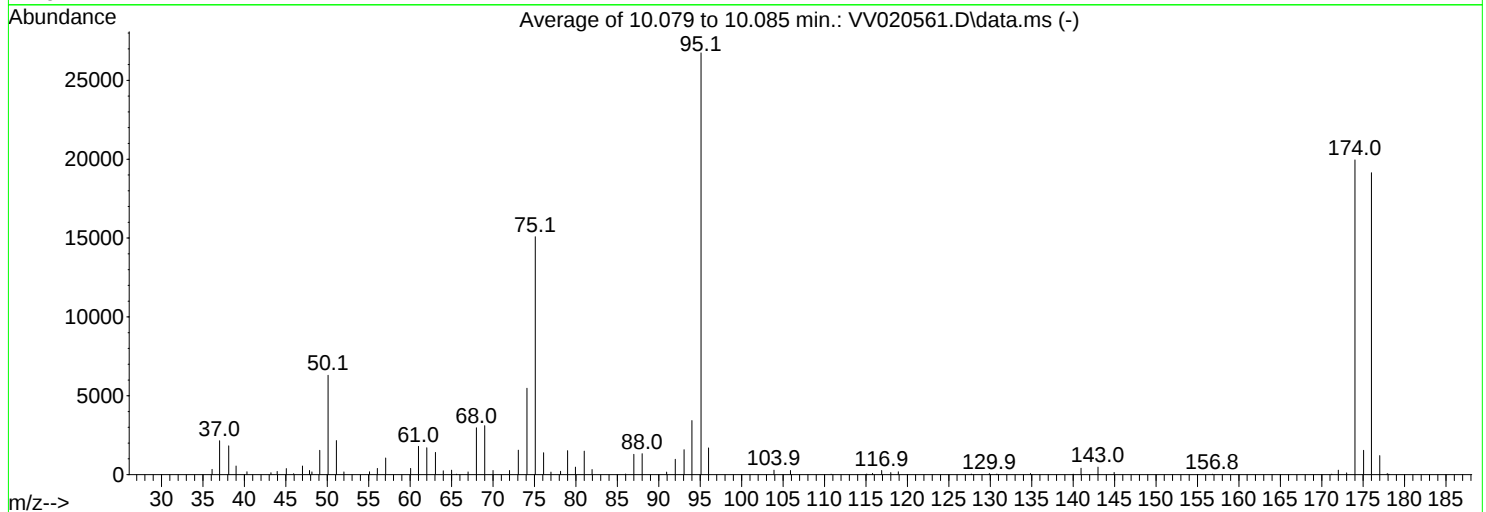


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031321\
 Data File : VV020561.D
 Acq On : 12 Mar 2021 12:21
 Operator : SY/MD
 Sample : BFB99
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB99

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Title : VOC Analysis
 Last Update : Sat Mar 13 02:32:38 2021

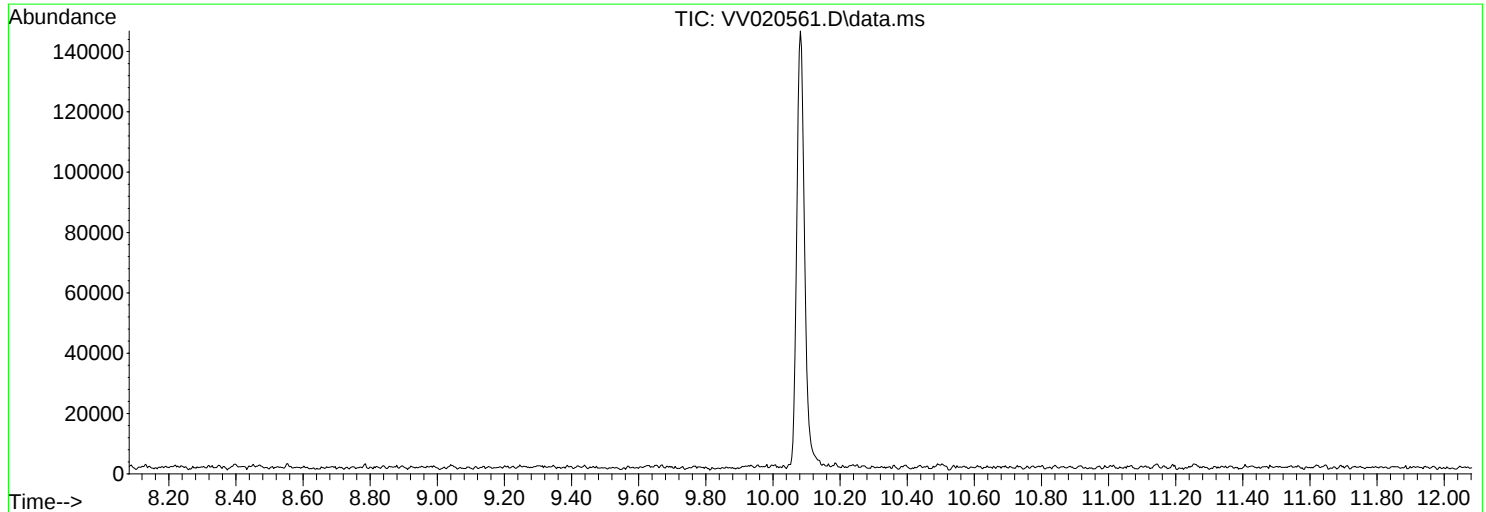

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	6299	PASS
75	95	30	80	56.4	15082	PASS
95	95	100	100	100.0	26744	PASS
96	95	5	9	6.3	1693	PASS
173	174	0.00	2	0.6	115	PASS
174	95	50	120	74.6	19960	PASS
175	174	5	9	7.7	1538	PASS
176	174	95	101	95.9	19141	PASS
177	176	5	9	6.3	1205	PASS

m/z	Abundance
36.20	464.0
37.00	2255.0
38.10	1794.0
39.10	664.0
39.90	165.0
40.30	172.0
41.30	111.0
42.60	116.0
43.30	115.0
44.00	520.0
45.10	443.0
46.00	168.0
47.00	462.0
47.80	289.0
48.20	261.0
49.10	1549.0
50.10	6267.0
51.10	2284.0
52.00	193.0
55.10	164.0
56.10	445.0
57.00	988.0
60.00	373.0
61.00	1858.0
62.10	1804.0
63.10	1395.0
64.00	260.0
65.00	289.0
65.60	102.0
67.00	211.0
68.00	3039.0
69.00	3084.0
70.00	275.0
72.00	248.0
73.00	1528.0
74.10	5273.0
75.10	15055.0
76.10	1474.0
77.00	260.0
78.10	203.0
79.00	1497.0
79.90	448.0
81.00	1441.0
82.00	303.0
87.00	1200.0
88.00	1293.0
91.00	162.0
92.00	1032.0
93.10	1479.0
94.00	3540.0
95.10	25920.0
96.00	1802.0
103.90	272.0
105.90	246.0
110.80	100.0
116.90	274.0
118.10	130.0
118.80	197.0
134.90	105.0
140.90	384.0
143.00	512.0
145.10	134.0
172.00	261.0
174.00	19280.0
175.00	1584.0
176.00	18712.0
177.00	1148.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.10	473.0
37.00	2288.0
38.10	1880.0
39.10	686.0
39.90	176.0
40.30	182.0
41.30	125.0
43.20	116.0
44.00	507.0
45.10	379.0
46.00	191.0
47.00	575.0
47.80	267.0
48.10	262.0
49.10	1584.0
50.10	6514.0
51.10	2216.0
52.00	189.0
55.10	196.0
56.10	540.0
57.00	1101.0
60.10	421.0
61.00	1840.0
62.10	1896.0
63.10	1469.0
64.00	242.0
65.00	286.0
67.00	173.0
68.00	3024.0
69.00	3207.0
70.00	276.0
72.00	265.0
73.00	1583.0
74.10	5654.0
75.10	15646.0
76.10	1411.0
77.00	292.0
78.20	212.0
79.00	1592.0
80.00	462.0
81.00	1552.0
82.00	316.0
86.00	107.0
87.00	1326.0
88.00	1333.0
91.00	155.0
92.00	989.0
93.10	1674.0
94.00	3578.0
95.10	27736.0
96.00	1727.0
103.90	312.0
105.90	274.0
115.80	115.0
116.90	271.0
118.00	129.0
118.90	179.0
129.90	110.0
140.90	410.0
143.00	491.0
144.90	140.0
156.80	106.0
172.00	288.0
174.00	20464.0
175.00	1529.0
176.00	19720.0
177.00	1248.0
177.90	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.10	468.0
37.00	1903.0
38.10	1802.0
39.00	742.0
39.90	177.0
40.30	180.0
41.30	149.0
43.10	139.0
44.00	455.0
45.00	327.0
46.00	189.0
47.00	596.0
47.90	251.0
49.10	1497.0
50.10	6115.0
51.10	1978.0
52.00	144.0
55.10	178.0
56.10	585.0
57.10	1080.0
60.10	391.0
61.00	1676.0
62.00	1782.0
63.00	1373.0
64.00	214.0
65.00	272.0
67.10	120.0
68.00	2856.0
69.00	3029.0
70.00	236.0
72.00	273.0
73.10	1544.0
74.10	5504.0
75.10	14546.0
76.10	1284.0
77.00	292.0
78.20	226.0
79.00	1493.0
80.00	508.0
81.00	1475.0
81.90	368.0
87.00	1335.0
88.00	1351.0
90.90	169.0
92.00	917.0
93.00	1596.0
94.10	3465.0
95.10	26576.0
96.00	1549.0
103.90	283.0
105.90	273.0
115.10	111.0
115.80	132.0
116.90	238.0
117.90	124.0
119.00	184.0
127.70	111.0
129.90	116.0
130.80	109.0
134.80	102.0
140.00	103.0
141.00	439.0
143.00	439.0
144.90	140.0
171.20	100.0
172.00	307.0
173.00	344.0
174.00	20136.0
175.10	1501.0
176.00	18992.0
177.00	1220.0
178.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.40	135.0
36.00	137.0
36.50	113.0
37.40	154.0
38.90	151.0
39.90	238.0
40.70	126.0
41.20	131.0
42.40	138.0
43.90	288.0
45.90	118.0
46.70	118.0
48.80	121.0
50.40	100.0
53.20	104.0
53.90	120.0
55.90	131.0
59.10	115.0
61.90	123.0
65.30	104.0
77.10	115.0
87.70	102.0
93.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99