




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030181.D
 Acq On : 13 Mar 2023 17:04
 Operator : SY/MD
 Sample : 01884-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB907

Manual IntegrationsAPPROVED

Quant Time: Mar 14 03:47:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 14 03:44:35 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/15/2023
 Supervised By :Mahesh Dadoda 03/15/2023

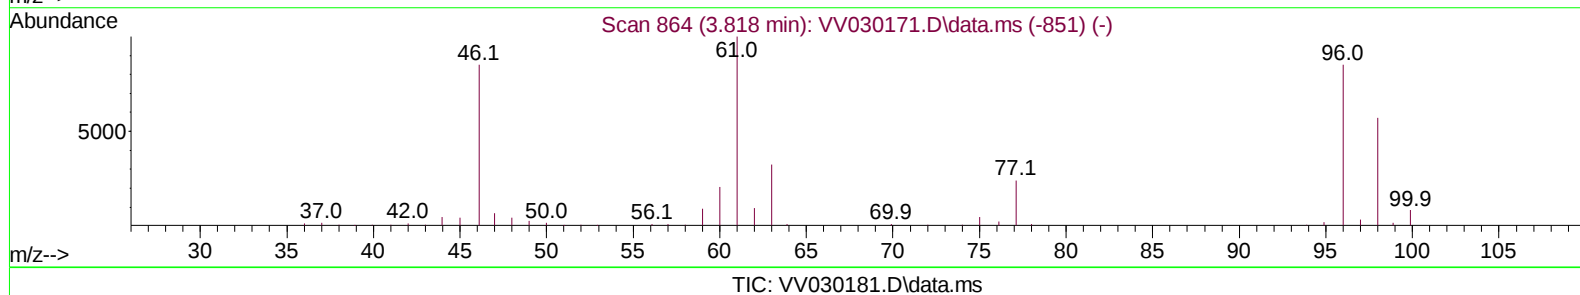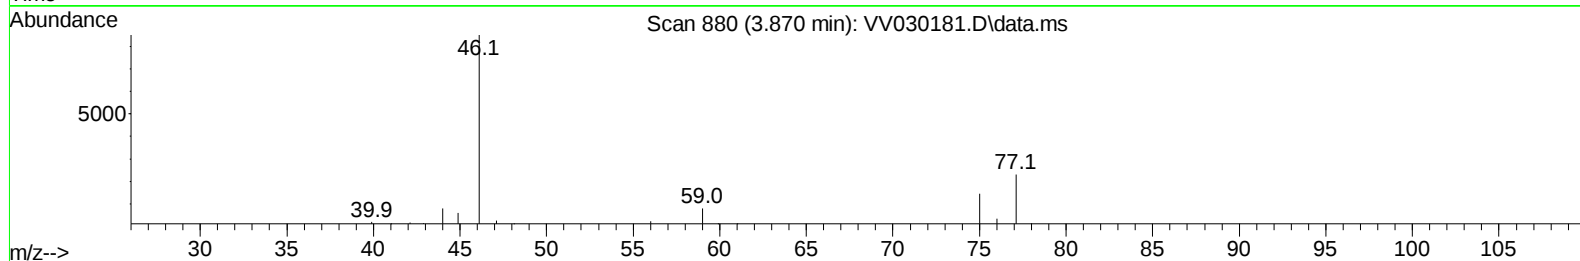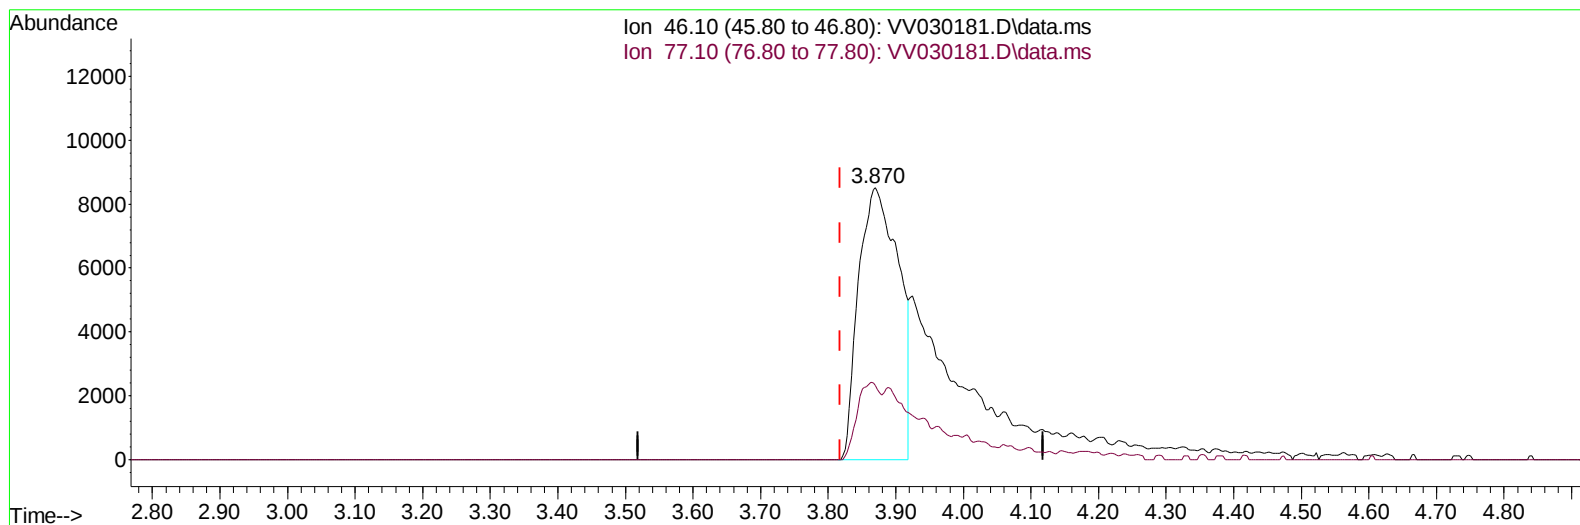

(20) 2-Butanone-d5 (S)

3.870min (+ 0.051) 20.32 ug/L

response 34859

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	16.47#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030181.D
 Acq On : 13 Mar 2023 17:04
 Operator : SY/MD
 Sample : 01884-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB907

Manual IntegrationsAPPROVED

Quant Time: Mar 14 03:47:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 14 03:44:35 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/15/2023
 Supervised By :Mahesh Dadoda 03/15/2023

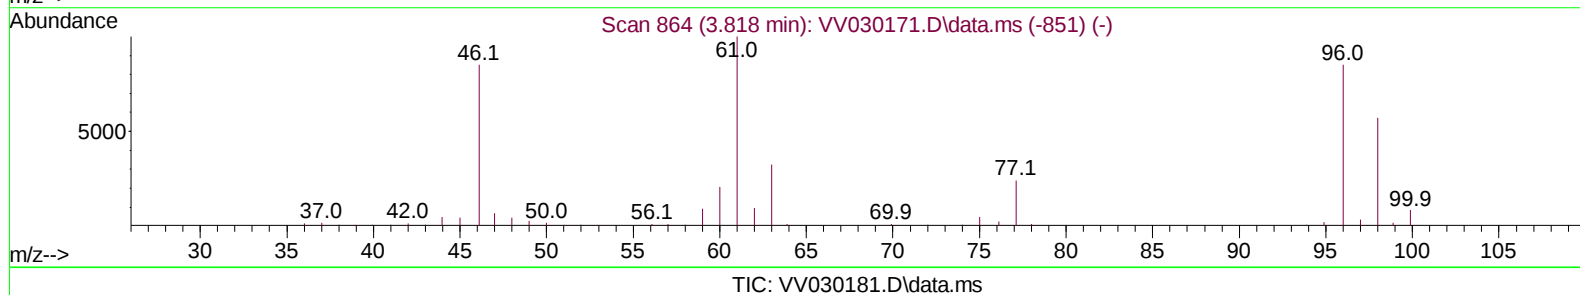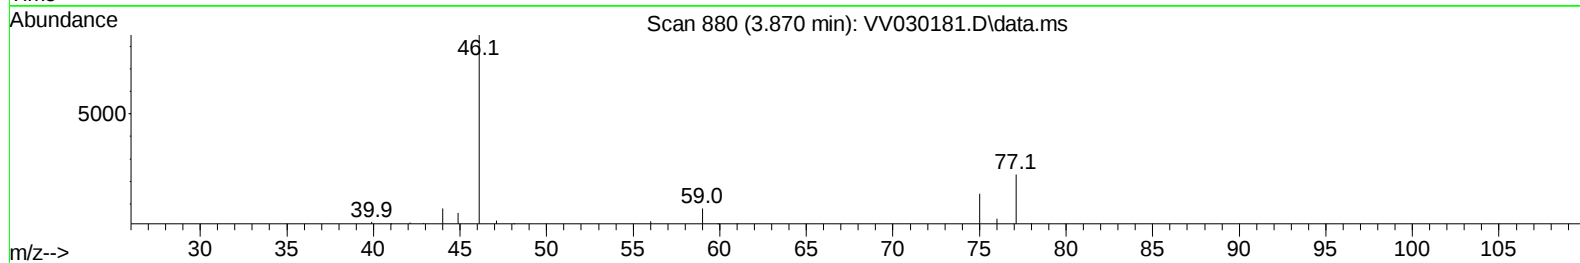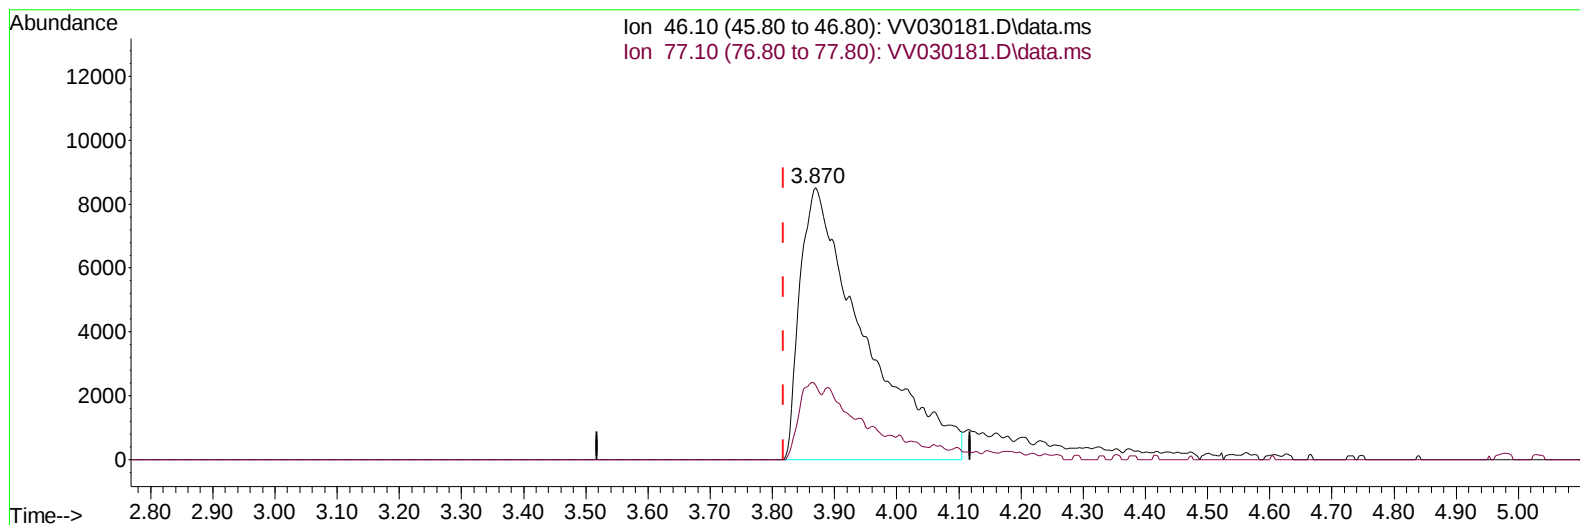

(20) 2-Butanone-d5 (S)

3.870min (+ 0.051) 35.61 ug/L m

response 61088

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	12.60	9.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030181.D
 Acq On : 13 Mar 2023 17:04
 Operator : SY/MD
 Sample : 01884-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB907

Manual IntegrationsAPPROVED

Quant Time: Mar 14 03:47:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 14 03:44:35 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/15/2023
 Supervised By :Mahesh Dadoda 03/15/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	143811	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	146546	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	78147	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	54941	5.904	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	118.000%	
7) Chloroethane-d5	1.535	69	46254	5.295	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	106.000%	
11) 1,1-Dichloroethene-d2	2.063	63	78478	4.102	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	82.000%	
20) 2-Butanone-d5	3.870	46	61088m	35.607	ug/L	0.05
Spiked Amount 50.000	Range 40	- 130	Recovery	=	71.220%	
24) Chloroform-d	4.262	84	94566	4.975	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	99.400%	
26) 1,2-Dichloroethane-d4	4.957	65	40112	5.169	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	103.400%	
32) Benzene-d6	4.973	84	179560	4.554	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.000%	
36) 1,2-Dichloropropane-d6	6.001	67	55488	4.677	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	93.600%	
41) Toluene-d8	7.252	98	156666	4.191	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	7.564	79	17756	4.375	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	87.400%	
46) 2-Hexanone-d5	8.040	63	62621	37.294	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	74.580%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	39213	4.646	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	11.570	152	67154	5.079	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	101.600%	
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.243	76	5161	0.200	ug/L #	94
17) Methyl tert-butyl Ether	2.722	73	7522	0.399	ug/L #	90
51) Chlorobenzene	8.825	112	23525	0.805	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030181.D
Acq On : 13 Mar 2023 17:04
Operator : SY/MD
Sample : 01884-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB907

Manual IntegrationsAPPROVED

Quant Time: Mar 14 03:47:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 14 03:44:35 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/15/2023
Supervised By :Mahesh Dadoda 03/15/2023

