

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030174.D
 Acq On : 13 Mar 2023 14:17
 Operator : SY/MD
 Sample : 01884-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB906

Quant Time: Mar 14 03:45:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 14 03:44:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	151259	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	153020	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	77353	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	57108	5.835	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.600%
7) Chloroethane-d5	1.539	69	48199	5.246	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.000%
11) 1,1-Dichloroethene-d2	2.066	63	80305	3.991	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.800%
20) 2-Butanone-d5	3.818	46	82001	45.443	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.880%
24) Chloroform-d	4.262	84	102320	5.118	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%
26) 1,2-Dichloroethane-d4	4.953	65	43244	5.298	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.000%
32) Benzene-d6	4.973	84	190545	4.628	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
36) 1,2-Dichloropropane-d6	5.998	67	59738	4.823	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.400%
41) Toluene-d8	7.252	98	169544	4.344	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.800%
43) trans-1,3-Dichloroprop...	7.561	79	20651	4.873	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.400%
46) 2-Hexanone-d5	8.037	63	72076	41.109	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.220%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	43339	4.918	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	11.571	152	66173	5.056	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds					Qvalue	
13) Acetone	2.146	43	4142	3.106	ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030174.D
Acq On : 13 Mar 2023 14:17
Operator : SY/MD
Sample : 01884-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB906

Quant Time: Mar 14 03:45:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 14 03:44:35 2023
Response via : Initial Calibration

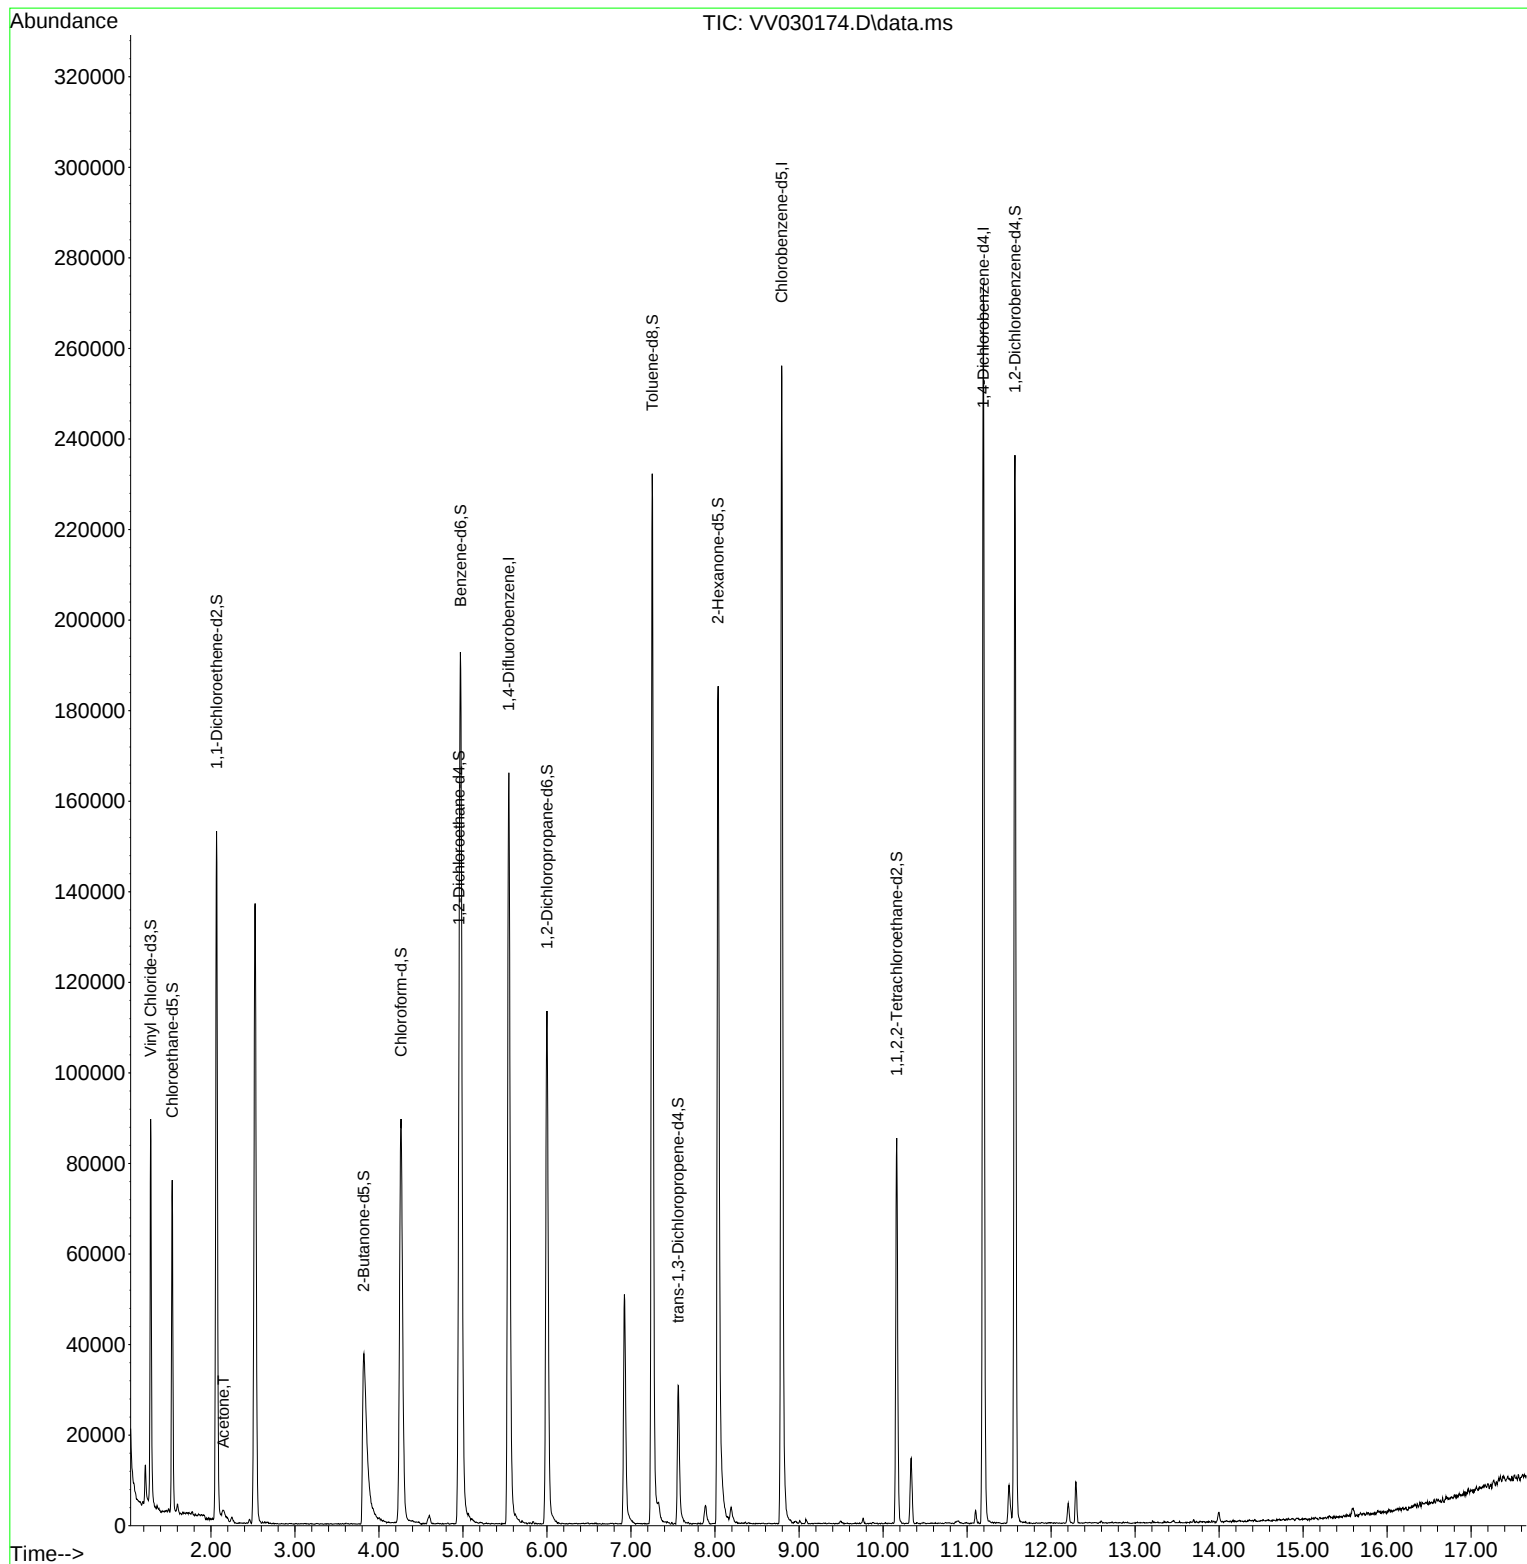

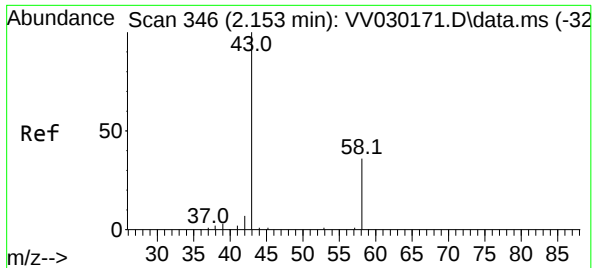

#13
 Acetone
 Concen: 3.106 ug/L
 RT: 2.146 min Scan# 34
 Delta R.T. -0.006 min
 Lab File: VV030174.D
 Acq: 13 Mar 2023 14:17

Instrument :
 MSVOA_V
 ClientSampleId :
 CB906

Tgt Ion: 43 Resp: 4142
 Ion Ratio Lower Upper
 43 100
 58 30.9 0.0 29.4#

