

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030184.D
 Acq On : 13 Mar 2023 18:17
 Operator : SY/MD
 Sample : 01868-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Mar 14 03:48:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 14 03:44:35 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.545	114	158387	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.792	117	153737	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.194	152	76990	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.281	65	61522	6.003	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	120.000%	
7) Chloroethane-d5		1.539	69	52616	5.469	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.400%	
11) 1,1-Dichloroethene-d2		2.066	63	86795	4.119	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.400%	
20) 2-Butanone-d5		3.818	46	87076	46.084	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.160%	
24) Chloroform-d		4.262	84	108984	5.206	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.200%	
26) 1,2-Dichloroethane-d4		4.953	65	46761	5.472	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.400%	
32) Benzene-d6		4.973	84	212378	5.134	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%	
36) 1,2-Dichloropropane-d6		5.998	67	64909	5.216	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.400%	
41) Toluene-d8		7.252	98	183984	4.692	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%	
43) trans-1,3-Dichloroprop...		7.561	79	22142	5.200	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.000%	
46) 2-Hexanone-d5		8.037	63	79367	45.056	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.120%	
56) 1,1,2,2-Tetrachloroeth...		10.162	84	46229	5.221	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.400%	
66) 1,2-Dichlorobenzene-d4		11.570	152	69514	5.337	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.800%	
Target Compounds							
16) Methylene chloride		2.458	84	3491	0.269	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030184.D
Acq On : 13 Mar 2023 18:17
Operator : SY/MD
Sample : 01868-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Mar 14 03:48:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 14 03:44:35 2023
Response via : Initial Calibration

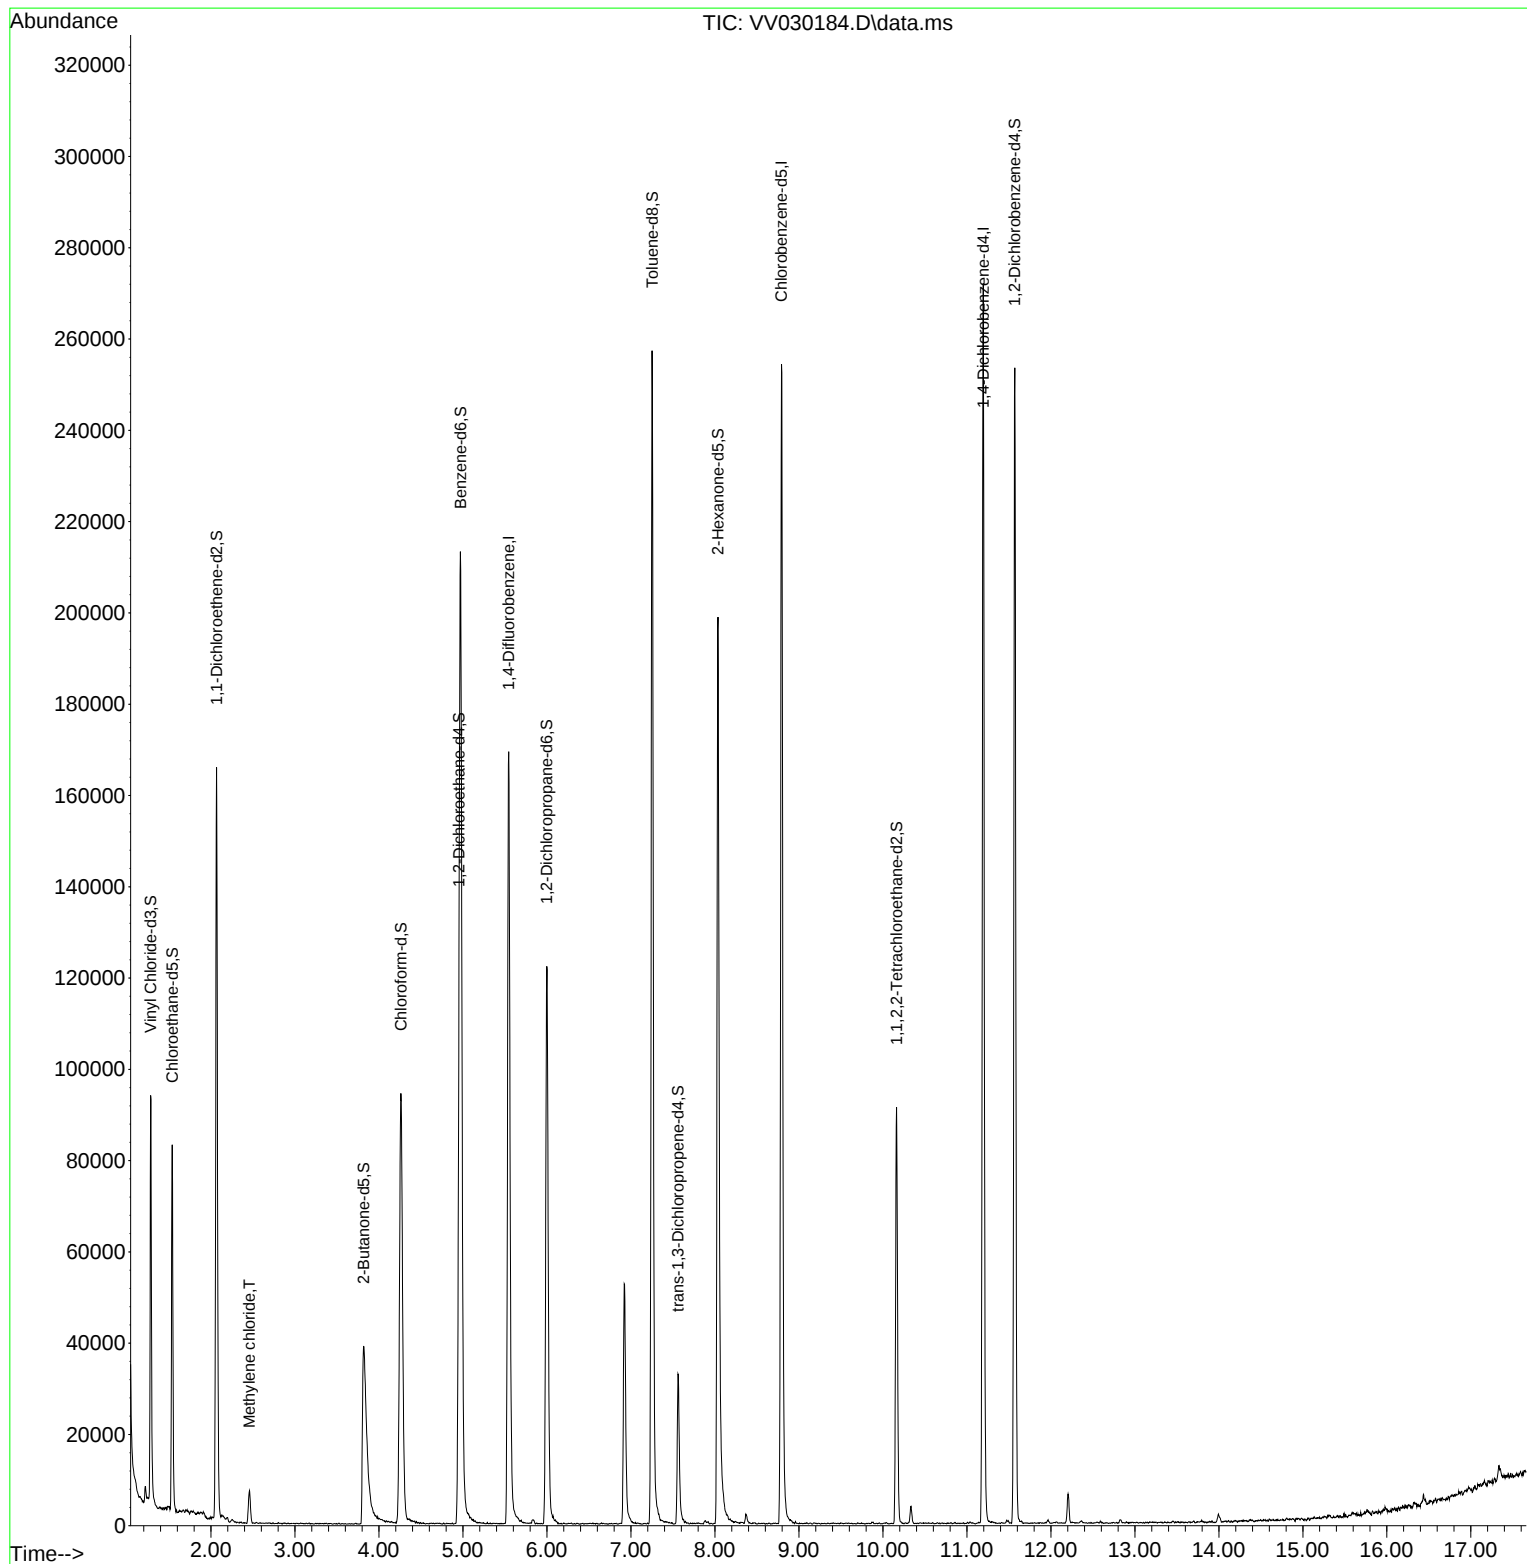

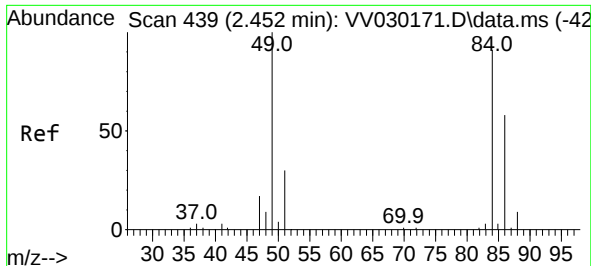

#16
Methylene chloride
Concen: 0.269 ug/L
RT: 2.458 min Scan# 441
Delta R.T. 0.006 min
Lab File: VV030184.D
Acq: 13 Mar 2023 18:17

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

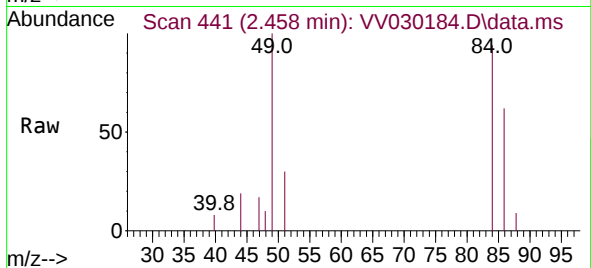

Tgt Ion: 84 Resp: 3491

Ion	Ratio	Lower	Upper
84	100		
86	65.8	44.7	83.1
49	106.8	78.8	146.3

