

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030172.D
 Acq On : 13 Mar 2023 13:28
 Operator : SY/MD
 Sample : VV0313WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK310

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	65	rBV2	3726	5408	1.09%	0.131%
2	1.281	69	75	94	rVB	87476	96935	19.50%	2.346%
3	1.539	147	155	168	rVB	77498	87774	17.66%	2.124%
4	2.066	308	319	334	rBV	155842	227247	45.72%	5.500%
5	2.458	432	441	453	rVB3	5243	8593	1.73%	0.208%
6	3.828	855	867	898	rBV2	34822	135054	27.17%	3.269%
7	4.265	986	1003	1026	rBV	88638	226056	45.48%	5.471%
8	4.973	1205	1223	1252	rBV2	196342	497014	100.00%	12.029%
9	5.545	1387	1401	1428	rBV	162748	334456	67.29%	8.095%
10	6.002	1525	1543	1575	rBV	114054	239343	48.16%	5.793%
11	6.924	1819	1830	1847	rBV	51645	96601	19.44%	2.338%
12	7.252	1919	1932	1967	rBV	236738	426353	85.78%	10.319%
13	7.564	2018	2029	2046	rBV	31248	56648	11.40%	1.371%
14	8.037	2165	2176	2207	rBV	188991	356293	71.69%	8.623%
15	8.792	2399	2411	2437	rBV	246428	411071	82.71%	9.949%
16	10.162	2825	2837	2852	rBV	87918	136882	27.54%	3.313%
17	11.194	3147	3158	3181	rBV	257741	407944	82.08%	9.874%
18	11.570	3263	3275	3294	rBV	236077	372291	74.91%	9.011%
19	12.204	3462	3472	3481	rVB	6501	9728	1.96%	0.235%




Sum of corrected areas: 4131691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030172.D
Acq On : 13 Mar 2023 13:28
Operator : SY/MD
Sample : VV0313WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

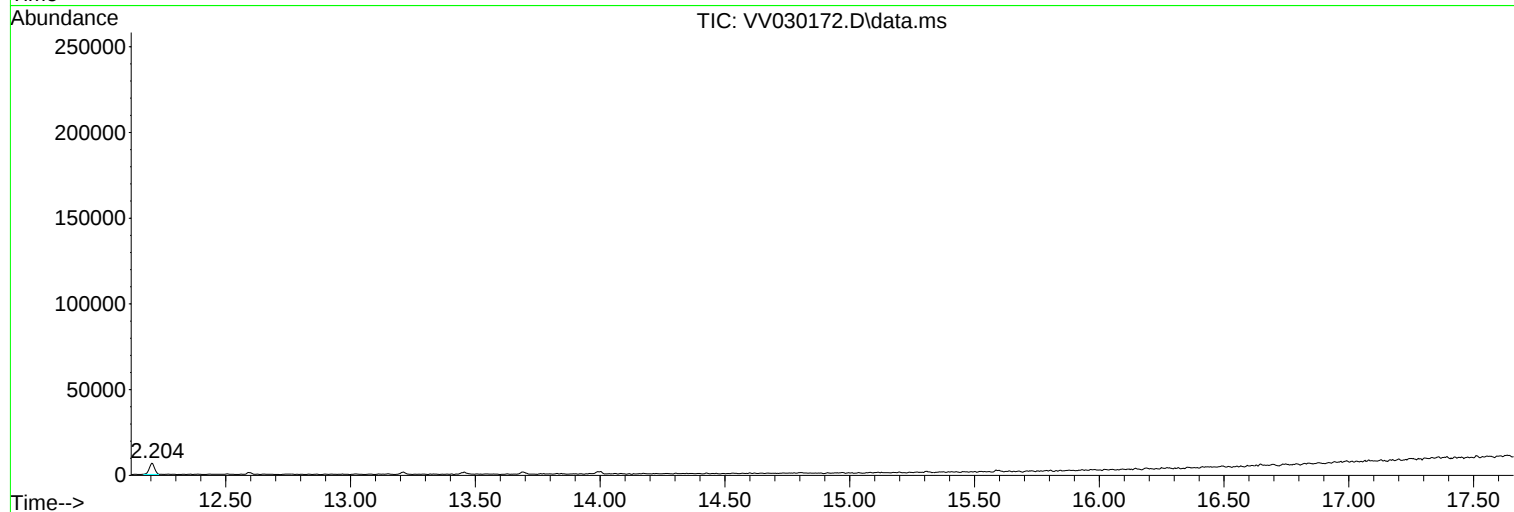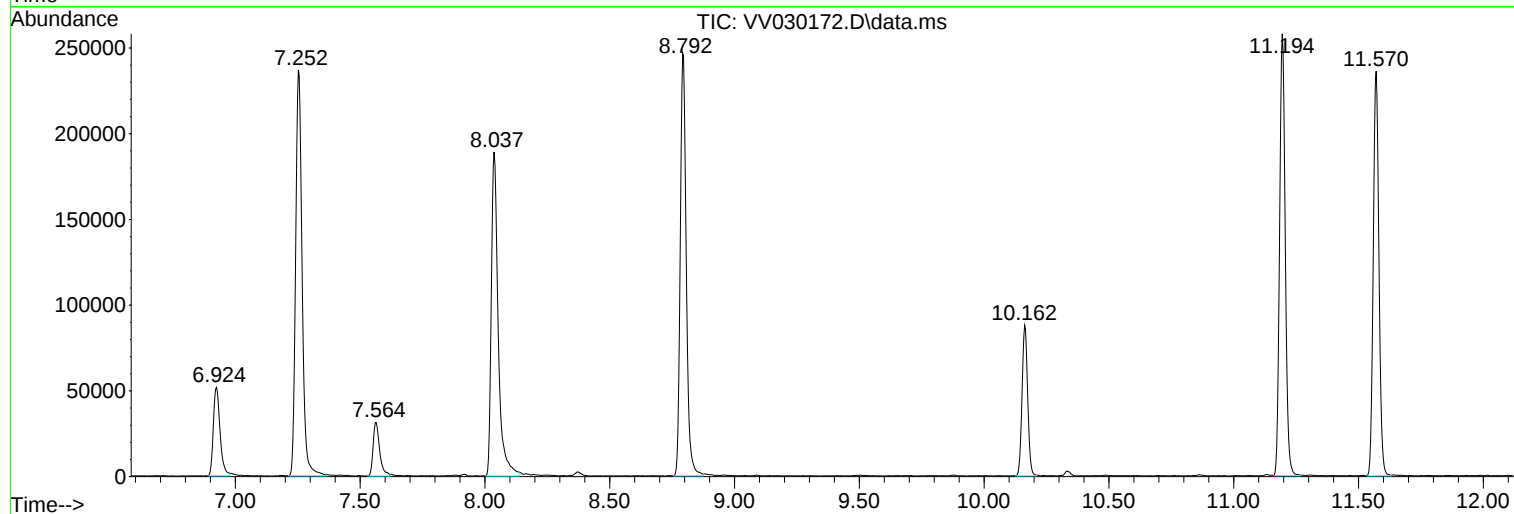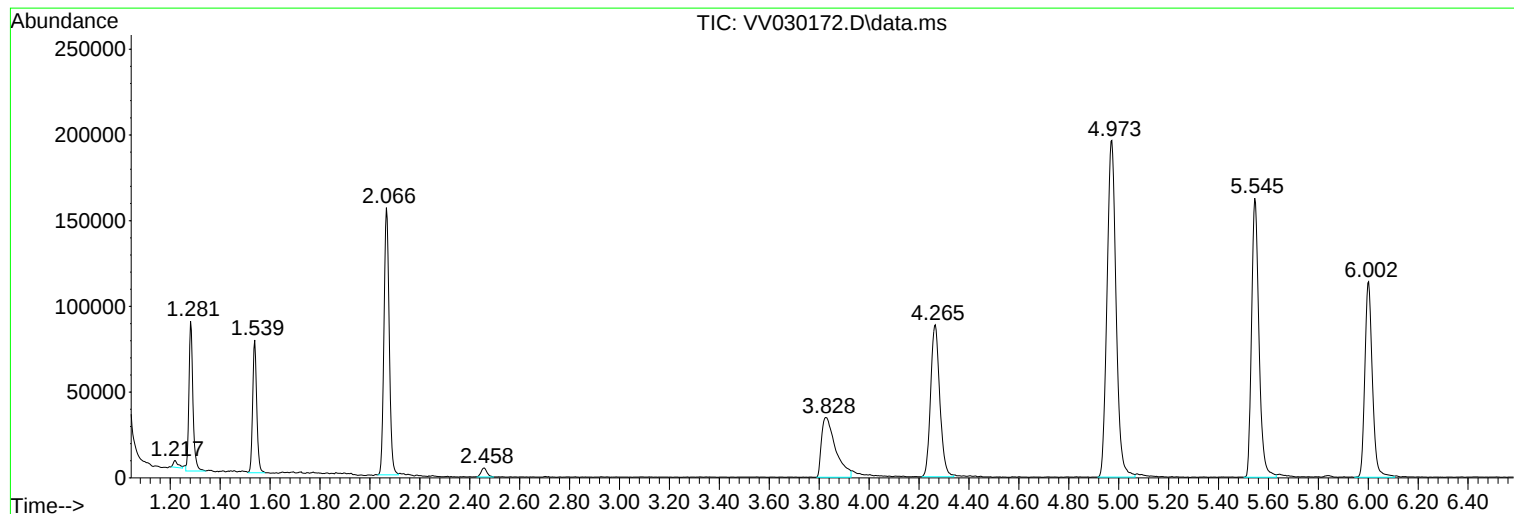

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030172.D
Acq On : 13 Mar 2023 13:28
Operator : SY/MD
Sample : VV0313WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030172.D
Acq On : 13 Mar 2023 13:28
Operator : SY/MD
Sample : VV0313WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------