

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030178.D
 Acq On : 13 Mar 2023 15:53
 Operator : SY/MD
 Sample : 01884-02DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB907DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	95	rVB	82519	91370	19.71%	2.357%
2	1.536	147	154	168	rVB	72051	84171	18.16%	2.171%
3	2.063	308	318	337	rBV	150461	218928	47.23%	5.648%
4	2.455	432	440	452	rVB3	5565	9630	2.08%	0.248%
5	3.847	860	873	905	rBV2	19358	101023	21.79%	2.606%
6	4.262	984	1002	1026	rBV	82214	211050	45.53%	5.444%
7	4.970	1203	1222	1248	rBV3	184214	463535	100.00%	11.958%
8	5.545	1387	1401	1430	rBV	154451	322377	69.55%	8.316%
9	5.998	1529	1542	1568	rBV2	105186	220391	47.55%	5.685%
10	6.921	1819	1829	1845	rBV	46045	85116	18.36%	2.196%
11	7.252	1919	1932	1962	rBV	221599	391494	84.46%	10.099%
12	7.561	2014	2028	2052	rBV	28377	52597	11.35%	1.357%
13	7.889	2117	2130	2136	rBV3	3132	5747	1.24%	0.148%
14	8.040	2166	2177	2217	rBV	153120	327445	70.64%	8.447%
15	8.793	2400	2411	2431	rBV	238052	400841	86.47%	10.340%
16	10.162	2825	2837	2857	rBV	80869	129570	27.95%	3.342%
17	10.333	2876	2890	2904	rBV	7603	12954	2.79%	0.334%
18	11.194	3146	3158	3179	rBV	254208	393843	84.97%	10.160%
19	11.571	3261	3275	3291	rBV	215519	336952	72.69%	8.692%
20	12.204	3462	3472	3482	rVB2	7411	11407	2.46%	0.294%
21	13.995	4021	4029	4041	rVB2	3835	6040	1.30%	0.156%




Sum of corrected areas: 3876481

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030178.D
Acq On : 13 Mar 2023 15:53
Operator : SY/MD
Sample : 01884-02DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB907DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

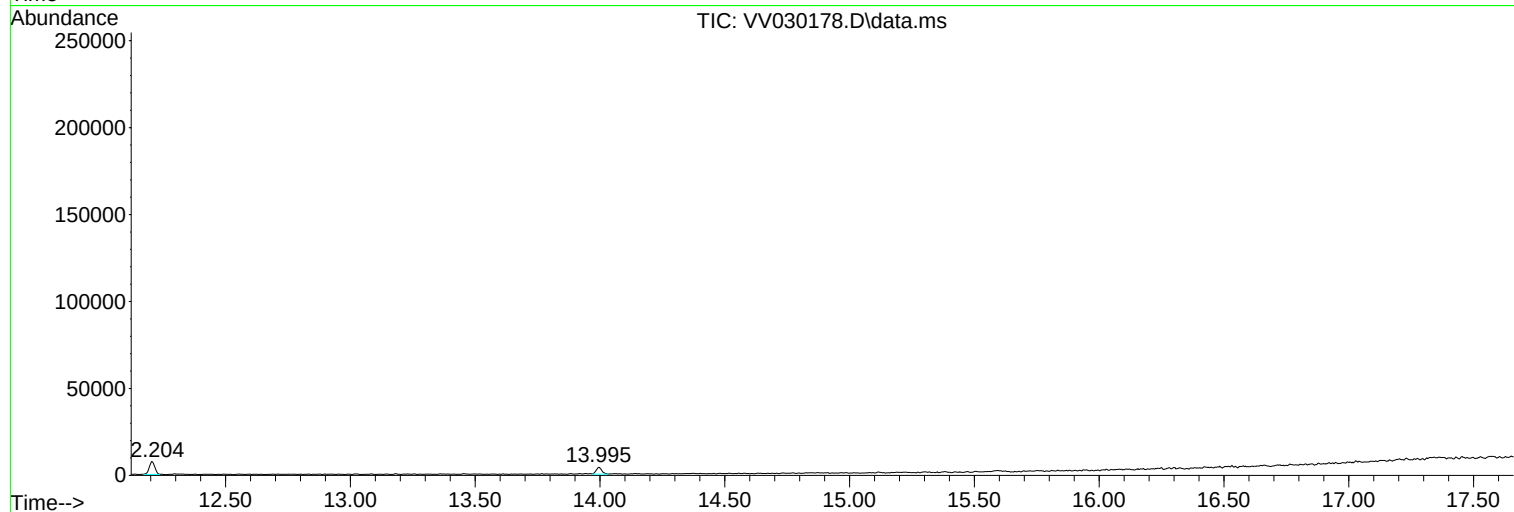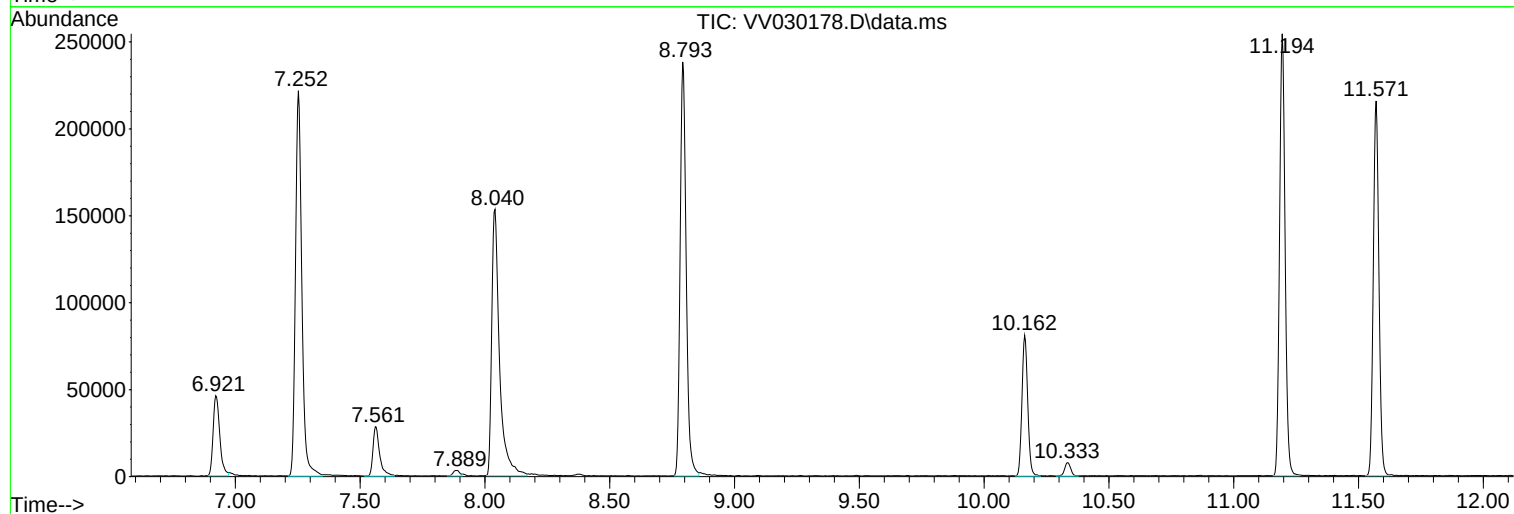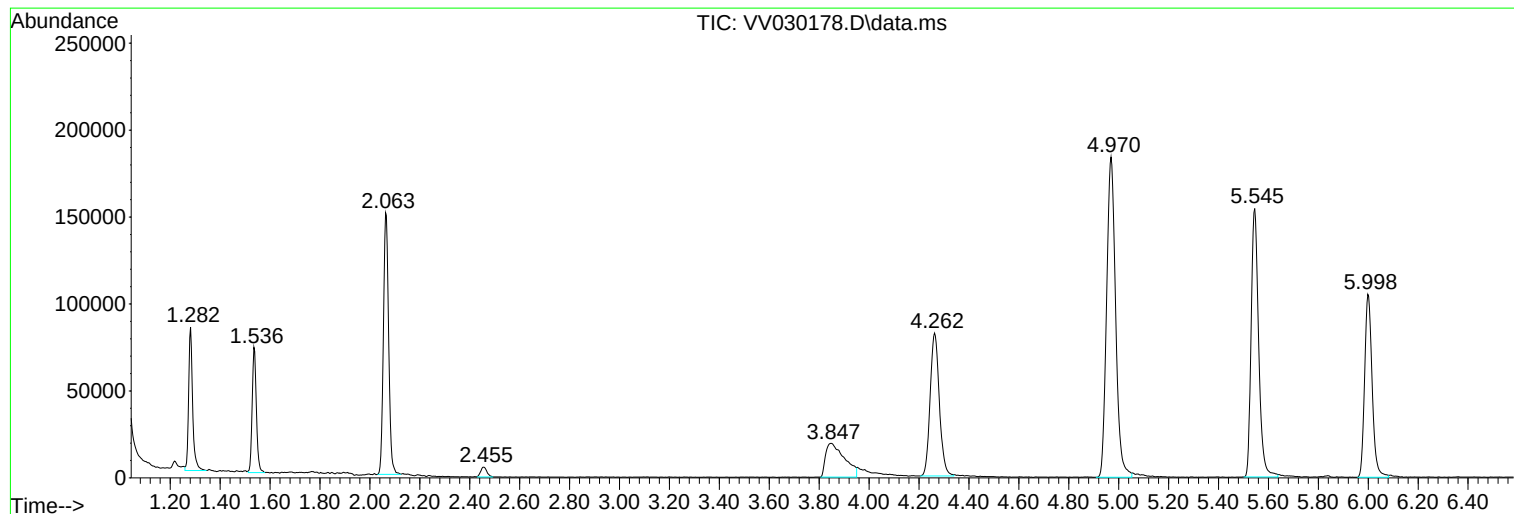

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030178.D
Acq On : 13 Mar 2023 15:53
Operator : SY/MD
Sample : 01884-02DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB907DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030178.D
Acq On : 13 Mar 2023 15:53
Operator : SY/MD
Sample : 01884-02DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB907DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc