

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030179.D
 Acq On : 13 Mar 2023 16:15
 Operator : SY/MD
 Sample : 01884-03DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB908DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	63	rBV3	3643	4992	1.10%	0.130%
2	1.281	68	75	95	rVB	81730	90840	19.95%	2.371%
3	1.539	147	155	171	rVB	71346	83125	18.26%	2.169%
4	2.066	309	319	336	rBV	147405	213846	46.97%	5.581%
5	2.458	428	441	451	rBV	5916	9679	2.13%	0.253%
6	3.838	856	870	909	rBV2	28581	125486	27.56%	3.275%
7	4.265	983	1003	1028	rBV2	82599	212370	46.65%	5.543%
8	4.973	1203	1223	1247	rBV3	179973	455274	100.00%	11.882%
9	5.545	1388	1401	1424	rBV	147998	301527	66.23%	7.870%
10	6.001	1529	1543	1574	rBV	102823	218231	47.93%	5.696%
11	6.924	1818	1830	1857	rBV2	46504	88056	19.34%	2.298%
12	7.252	1920	1932	1969	rBV	212492	383411	84.22%	10.007%
13	7.564	2019	2029	2048	rBV2	28536	51300	11.27%	1.339%
14	8.037	2166	2176	2208	rBV	169114	327417	71.92%	8.545%
15	8.796	2400	2412	2444	rBV	227384	399559	87.76%	10.428%
16	10.162	2825	2837	2853	rBV	81754	127470	28.00%	3.327%
17	11.194	3146	3158	3177	rBV	244027	377762	82.97%	9.859%
18	11.477	3235	3246	3249	rBV4	3363	5079	1.12%	0.133%
19	11.570	3263	3275	3293	rBV	218705	341527	75.02%	8.913%
20	11.963	3390	3397	3404	rBV3	3815	5512	1.21%	0.144%
21	12.204	3461	3472	3484	rBV2	5346	9110	2.00%	0.238%




Sum of corrected areas: 3831573

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030179.D
Acq On : 13 Mar 2023 16:15
Operator : SY/MD
Sample : 01884-03DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB908DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

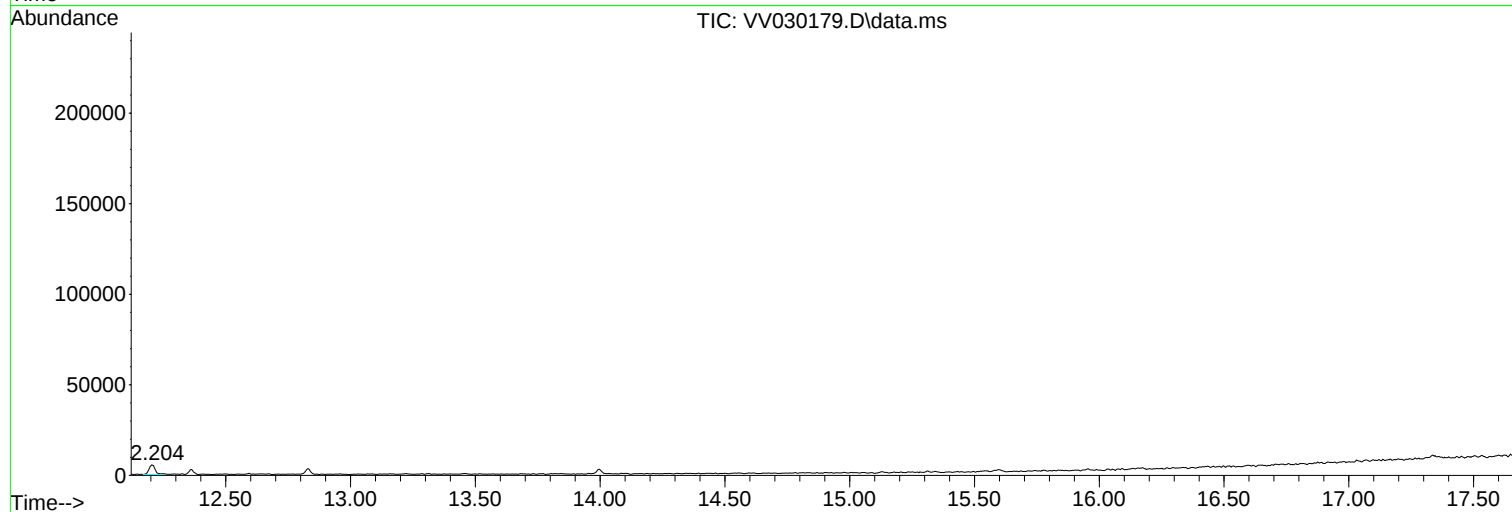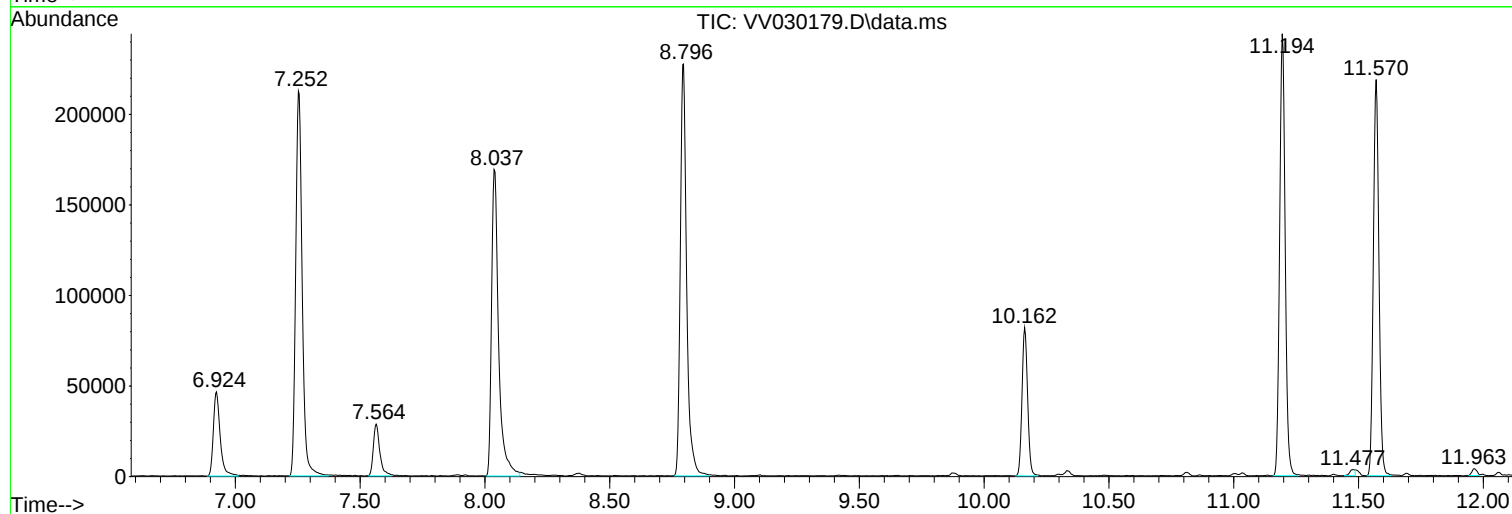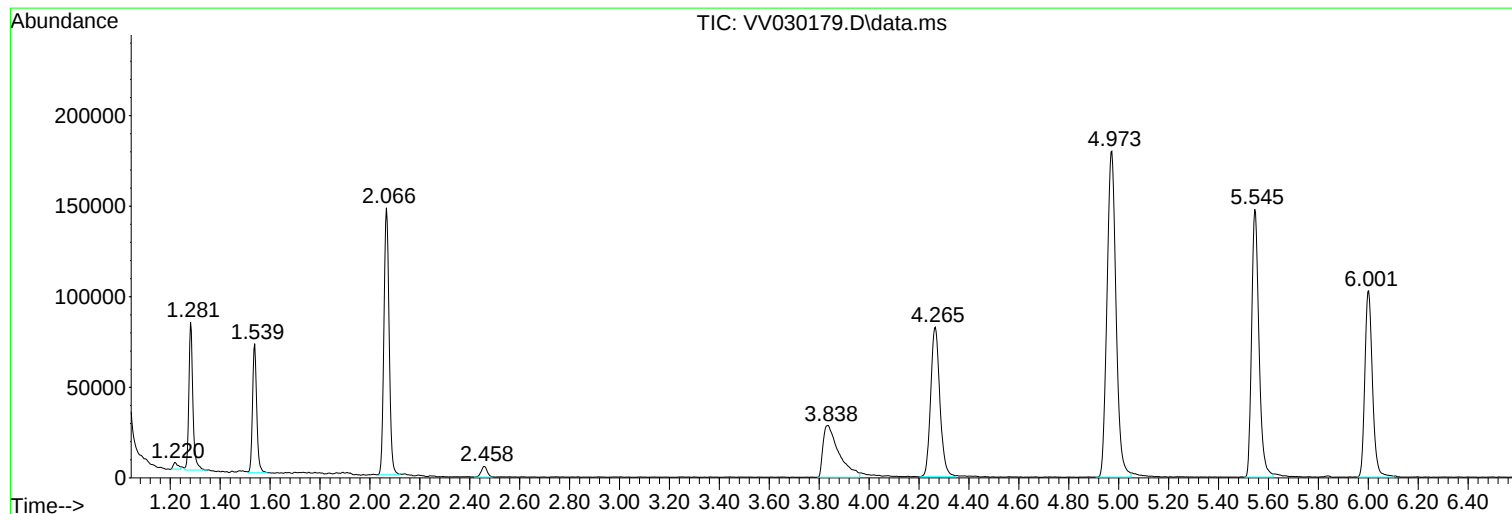

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030179.D
Acq On : 13 Mar 2023 16:15
Operator : SY/MD
Sample : 01884-03DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB908DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030179.D
Acq On : 13 Mar 2023 16:15
Operator : SY/MD
Sample : 01884-03DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB908DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------