

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
 Data File : VV030184.D
 Acq On : 13 Mar 2023 18:17
 Operator : SY/MD
 Sample : 01868-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	98	rVB	90172	102634	19.22%	2.344%
2	1.539	147	155	169	rVB	80447	93390	17.49%	2.133%
3	2.066	309	319	335	rBV	164292	237608	44.50%	5.427%
4	2.458	431	441	452	rBV2	7206	12269	2.30%	0.280%
5	3.818	853	864	901	rBV	38852	142815	26.75%	3.262%
6	4.262	985	1002	1027	rBV	94069	243119	45.53%	5.553%
7	4.969	1205	1222	1248	rBV2	212938	533921	100.00%	12.195%
8	5.545	1388	1401	1430	rBV	169101	350370	65.62%	8.003%
9	5.998	1526	1542	1565	rBV	122145	253653	47.51%	5.793%
10	6.921	1819	1829	1858	rBV	52532	100880	18.89%	2.304%
11	7.252	1919	1932	1962	rBV	257072	457816	85.75%	10.457%
12	7.561	2013	2028	2046	rBV	32912	58937	11.04%	1.346%
13	8.037	2164	2176	2208	rBV	198633	378164	70.83%	8.637%
14	8.792	2399	2411	2433	rBV	254048	429559	80.45%	9.811%
15	10.162	2826	2837	2853	rBV	91199	144479	27.06%	3.300%
16	10.336	2883	2891	2904	rVB	3814	5640	1.06%	0.129%
17	11.194	3146	3158	3179	rBV	271570	425495	79.69%	9.718%
18	11.570	3263	3275	3289	rBV	253182	397142	74.38%	9.071%
19	12.204	3460	3472	3483	rBV2	6452	10365	1.94%	0.237%




Sum of corrected areas: 4378256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030184.D
Acq On : 13 Mar 2023 18:17
Operator : SY/MD
Sample : 01868-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

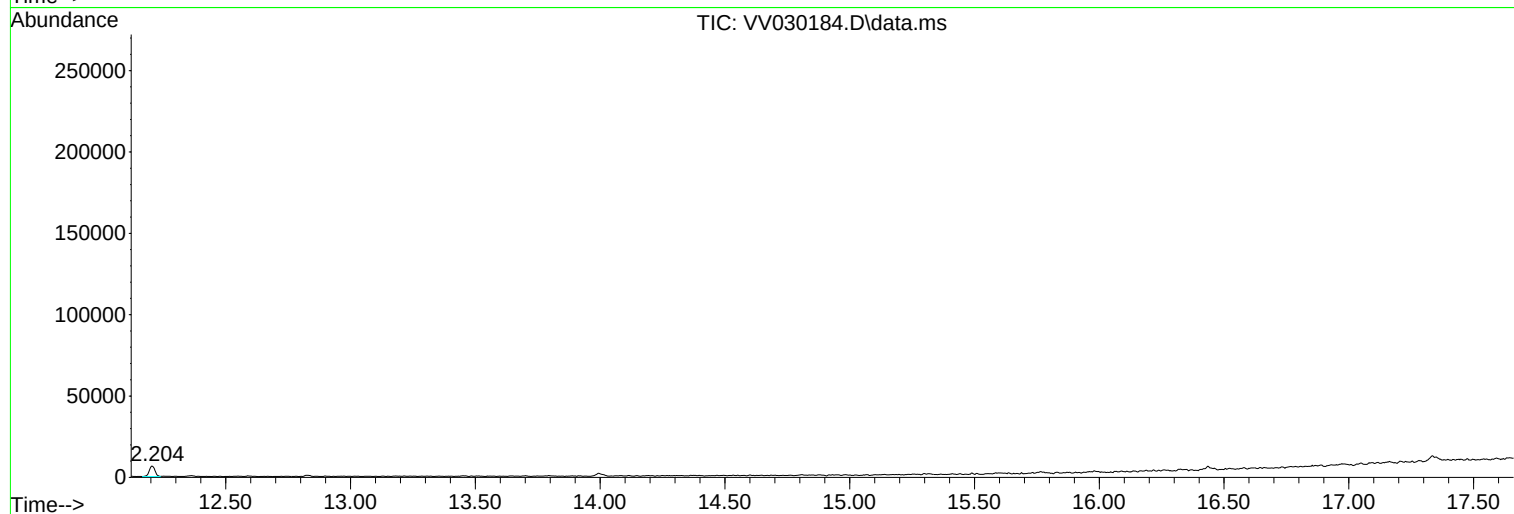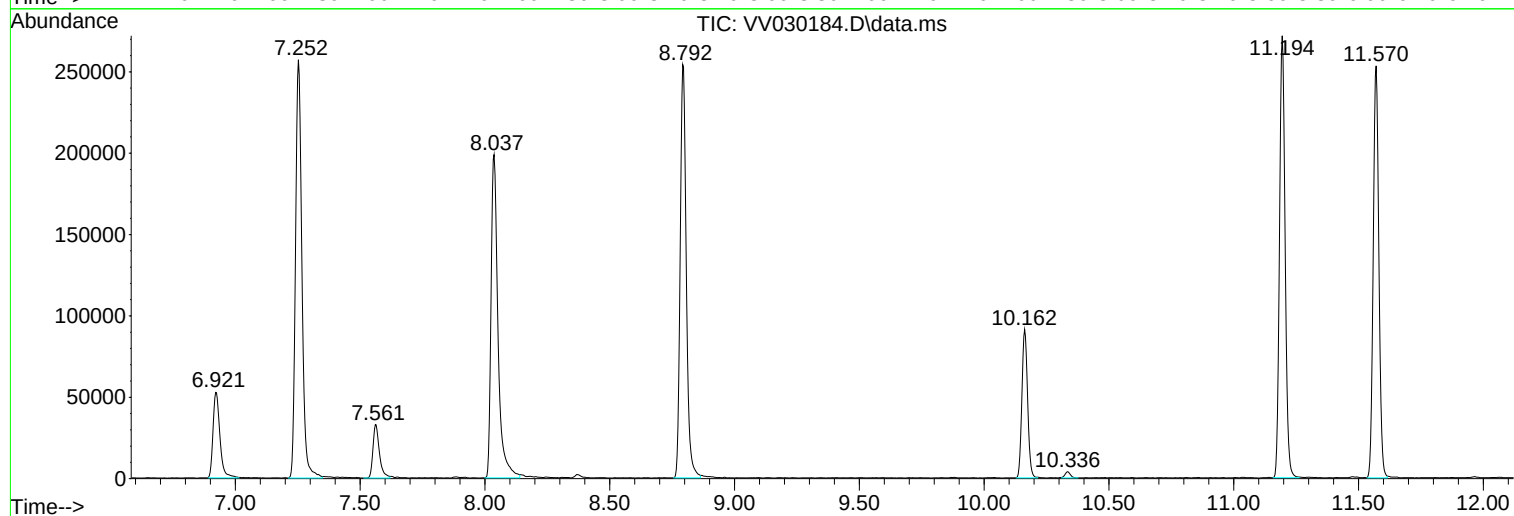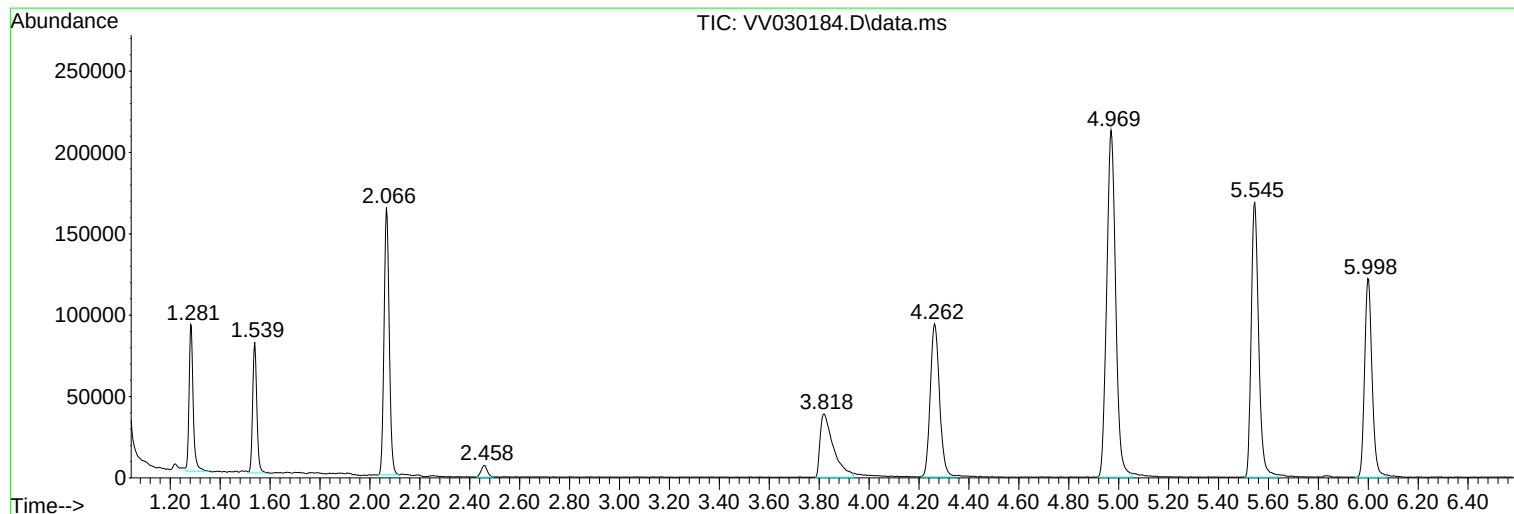

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030184.D
Acq On : 13 Mar 2023 18:17
Operator : SY/MD
Sample : 01868-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030184.D
Acq On : 13 Mar 2023 18:17
Operator : SY/MD
Sample : 01868-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc