


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031323\
Data File : VV030170.D
Acq On : 13 Mar 2023 11:04
Operator : SY/MD
Sample : BFB230
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB230

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Mar 14 03:44:35 2023

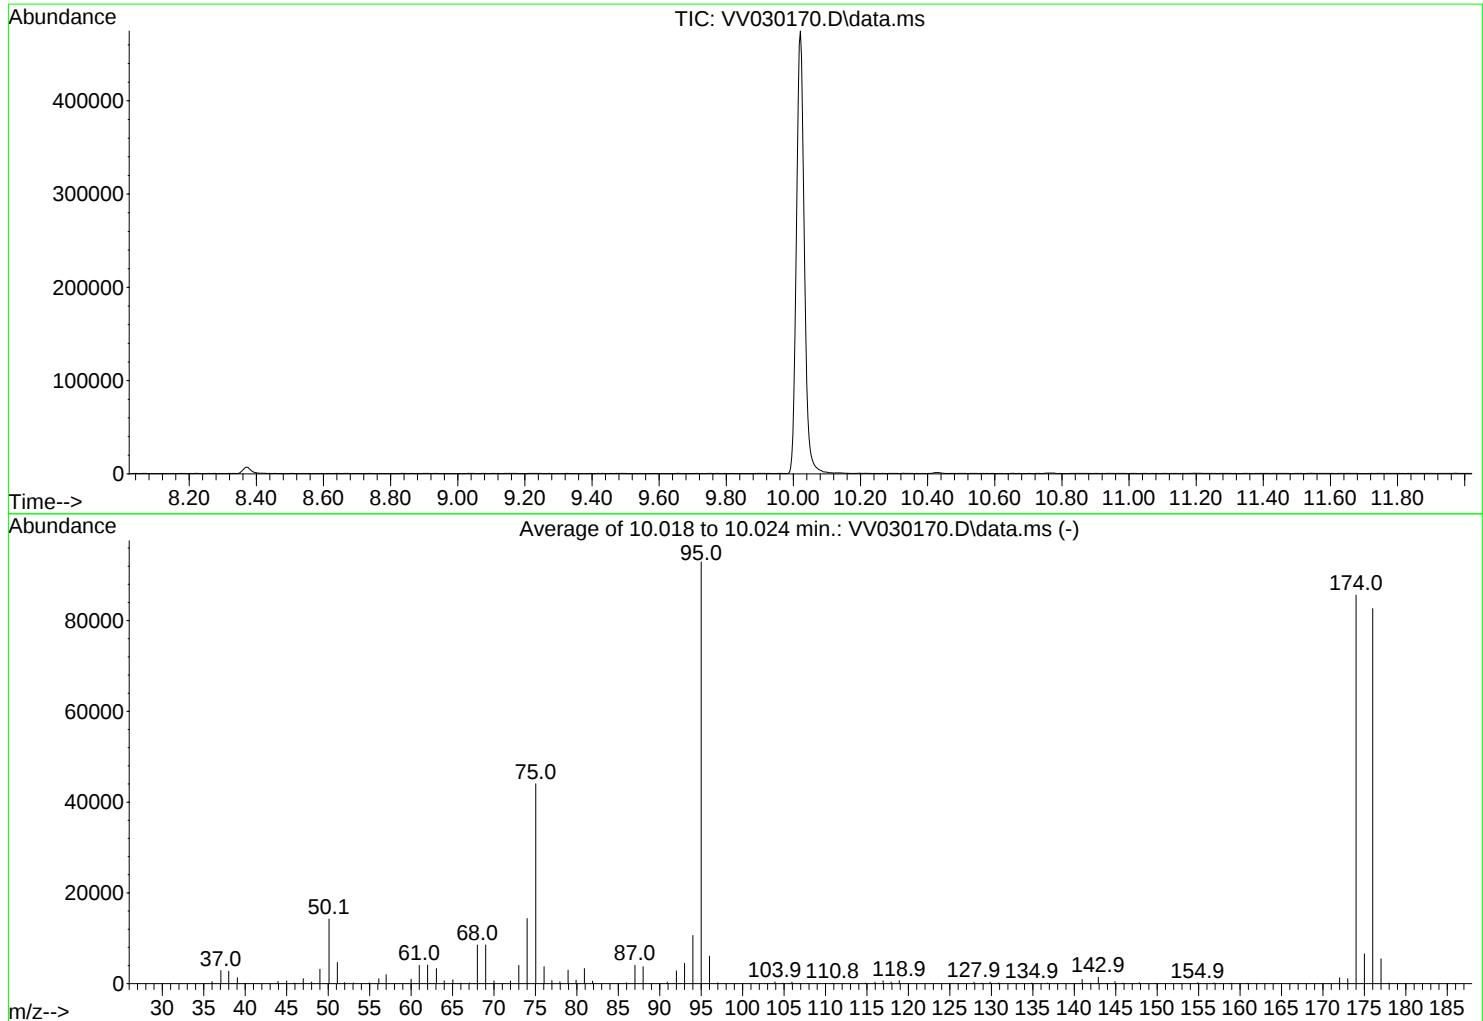

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	14247	PASS
75	95	30	80	47.4	44040	PASS
95	95	100	100	100.0	92947	PASS
96	95	5	9	6.5	6060	PASS
173	174	0.00	2	1.3	1106	PASS
174	95	50	120	92.1	85616	PASS
175	174	5	9	7.6	6548	PASS
176	174	95	105	96.5	82632	PASS
177	176	5	10	6.6	5453	PASS

m/z	Abundance
40.00	131.0
43.90	290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	507.0
37.10	2779.0
38.00	2752.0
39.00	1313.0
39.90	203.0
44.00	753.0
45.00	608.0
45.90	138.0
47.00	1099.0
48.00	351.0
49.00	3208.0
50.10	14652.0
51.10	4798.0
52.00	250.0
53.00	158.0
54.90	213.0
56.10	1008.0
57.00	1927.0
60.00	976.0
61.00	4226.0
62.00	4132.0
63.10	3408.0
64.00	560.0
65.00	848.0
66.00	134.0
67.00	172.0
68.00	8478.0
69.00	8918.0
70.00	633.0
72.00	548.0
73.00	4187.0
74.00	14738.0
75.00	44664.0
76.10	3891.0
77.00	675.0
78.00	406.0
79.00	3068.0
79.90	825.0
80.90	3327.0
81.90	583.0
86.10	205.0
87.00	4125.0
88.00	3675.0
90.90	373.0
92.00	2708.0
93.00	4460.0
94.00	10533.0
95.00	93232.0
96.00	6187.0
97.00	206.0
103.90	394.0
104.90	114.0
106.00	283.0
106.90	102.0
110.90	113.0
114.80	146.0
116.00	388.0
117.00	629.0
117.90	401.0
118.90	700.0
127.90	312.0
128.90	132.0
129.90	340.0
130.90	151.0
134.90	180.0
136.80	133.0
141.00	1001.0
141.90	163.0
142.90	1429.0
143.90	107.0
144.90	509.0
145.90	142.0
147.90	199.0
149.80	107.0
154.90	265.0
156.80	175.0
158.90	105.0
160.90	120.0
170.80	147.0
172.00	1179.0
173.00	1082.0
174.00	84400.0
175.00	6486.0
176.00	81440.0
177.00	5404.0
177.90	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	475.0
37.10	2961.0
38.00	2820.0
39.10	1361.0
39.90	219.0
44.00	799.0
45.00	610.0
45.90	164.0
47.00	1140.0
48.00	361.0
49.00	3328.0
50.10	14696.0
51.10	4860.0
52.00	247.0
53.00	173.0
54.90	203.0
56.10	1141.0
57.00	2048.0
60.00	1018.0
61.00	4157.0
62.00	4274.0
63.10	3460.0
64.00	659.0
65.10	849.0
66.00	144.0
67.10	186.0
68.00	8832.0
69.00	8833.0
70.00	668.0
72.00	573.0
73.00	4130.0
74.00	14857.0
75.00	45184.0
76.00	3861.0
77.00	712.0
78.00	437.0
79.00	3002.0
79.90	796.0
80.90	3400.0
81.90	555.0
86.00	201.0
87.00	4168.0
88.00	3835.0
90.90	390.0
92.00	2947.0
93.00	4718.0
94.00	10895.0
95.00	95648.0
96.00	6229.0
97.00	195.0
103.90	421.0
104.90	106.0
105.90	348.0
110.80	111.0
114.80	133.0
116.00	349.0
117.00	657.0
117.90	424.0
118.90	687.0
127.90	379.0
128.80	168.0
129.80	366.0
130.90	185.0
134.90	180.0
136.80	165.0
141.00	938.0
142.00	140.0
142.90	1445.0
144.90	470.0
145.80	148.0
147.80	232.0
149.80	100.0
152.80	101.0
154.90	255.0
156.80	165.0
158.90	112.0
160.90	121.0
172.00	1340.0
173.00	1124.0
174.00	88096.0
175.00	6774.0
176.00	85416.0
177.00	5638.0
178.00	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	420.0
37.00	2894.0
38.00	2661.0
39.10	1288.0
40.00	239.0
44.00	823.0
45.00	613.0
45.90	162.0
47.00	1056.0
48.00	357.0
49.00	3008.0
50.10	13393.0
51.10	4350.0
51.90	221.0
53.10	152.0
55.00	166.0
56.10	1097.0
57.00	1936.0
60.00	925.0
61.00	3718.0
62.00	3903.0
63.00	3124.0
64.00	645.0
65.10	810.0
66.00	155.0
67.10	173.0
68.00	8154.0
69.00	7892.0
70.00	660.0
72.00	538.0
73.00	3730.0
74.00	13463.0
75.10	42272.0
76.00	3501.0
77.00	636.0
77.90	425.0
78.90	2786.0
79.90	681.0
80.90	3182.0
81.90	508.0
85.90	184.0
87.00	3906.0
88.00	3707.0
90.90	329.0
92.00	2844.0
93.00	4277.0
94.00	10389.0
95.00	89960.0
96.00	5765.0
97.00	171.0
103.90	403.0
104.80	101.0
105.90	393.0
114.80	110.0
115.80	285.0
116.90	626.0
117.90	372.0
118.90	609.0
127.90	391.0
128.80	178.0
129.90	361.0
130.90	193.0
134.90	164.0
136.80	171.0
140.90	861.0
142.00	111.0
142.90	1387.0
144.90	397.0
145.90	134.0
146.80	101.0
147.80	261.0
152.80	113.0
154.90	234.0
156.90	165.0
158.90	106.0
160.80	113.0
172.00	1424.0
173.00	1113.0
174.00	84352.0
175.00	6385.0
176.00	81040.0
177.00	5318.0
178.00	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230