

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV031325\  
 Data File : VV038703.D  
 Acq On : 13 Mar 2025 14:59  
 Operator : SY/MD  
 Sample : VV0313WBL01  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR031325WMA.M  
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038703.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.275       | 66            | 73          | 87           | rBV      | 69096          | 76007         | 14.18%          | 1.729%        |
| 2         | 1.529       | 143           | 152         | 166          | rVV      | 68623          | 85214         | 15.90%          | 1.938%        |
| 3         | 2.053       | 305           | 315         | 328          | rBV      | 133365         | 191453        | 35.73%          | 4.355%        |
| 4         | 2.439       | 425           | 435         | 445          | rBV4     | 4092           | 7234          | 1.35%           | 0.165%        |
| 5         | 3.796       | 850           | 857         | 890          | rBV      | 51151          | 169805        | 31.69%          | 3.862%        |
| 6         | 4.240       | 977           | 995         | 1022         | rBV2     | 94223          | 251602        | 46.95%          | 5.723%        |
| 7         | 4.947       | 1203          | 1215        | 1252         | rBV3     | 200943         | 535876        | 100.00%         | 12.189%       |
| 8         | 5.526       | 1386          | 1395        | 1429         | rBV      | 167810         | 382319        | 71.34%          | 8.696%        |
| 9         | 5.979       | 1525          | 1536        | 1565         | rBV2     | 117671         | 269216        | 50.24%          | 6.123%        |
| 10        | 6.915       | 1818          | 1827        | 1853         | rBV2     | 36106          | 87622         | 16.35%          | 1.993%        |
| 11        | 7.236       | 1917          | 1927        | 1948         | rBV      | 195823         | 372117        | 69.44%          | 8.464%        |
| 12        | 7.561       | 2017          | 2028        | 2049         | rBV2     | 20777          | 48624         | 9.07%           | 1.106%        |
| 13        | 8.021       | 2163          | 2171        | 2213         | rBV      | 188846         | 471027        | 87.90%          | 10.714%       |
| 14        | 8.776       | 2397          | 2406        | 2439         | rBV      | 289794         | 524456        | 97.87%          | 11.929%       |
| 15        | 10.146      | 2819          | 2832        | 2849         | rBV      | 93960          | 160580        | 29.97%          | 3.652%        |
| 16        | 11.178      | 3143          | 3153        | 3181         | rBV      | 242189         | 418623        | 78.12%          | 9.522%        |
| 17        | 11.554      | 3258          | 3270        | 3293         | rBV      | 198055         | 344751        | 64.33%          | 7.841%        |




Sum of corrected areas: 4396

ABTKS84  
 Client Sample ID :  
 MSVOA\_V  
 Instrument :

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV031325\  
Data File : VV038703.D  
Acq On : 13 Mar 2025 14:59  
Operator : SY/MD  
Sample : VV0313WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 10 Sample Multiplier: 1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR031325WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

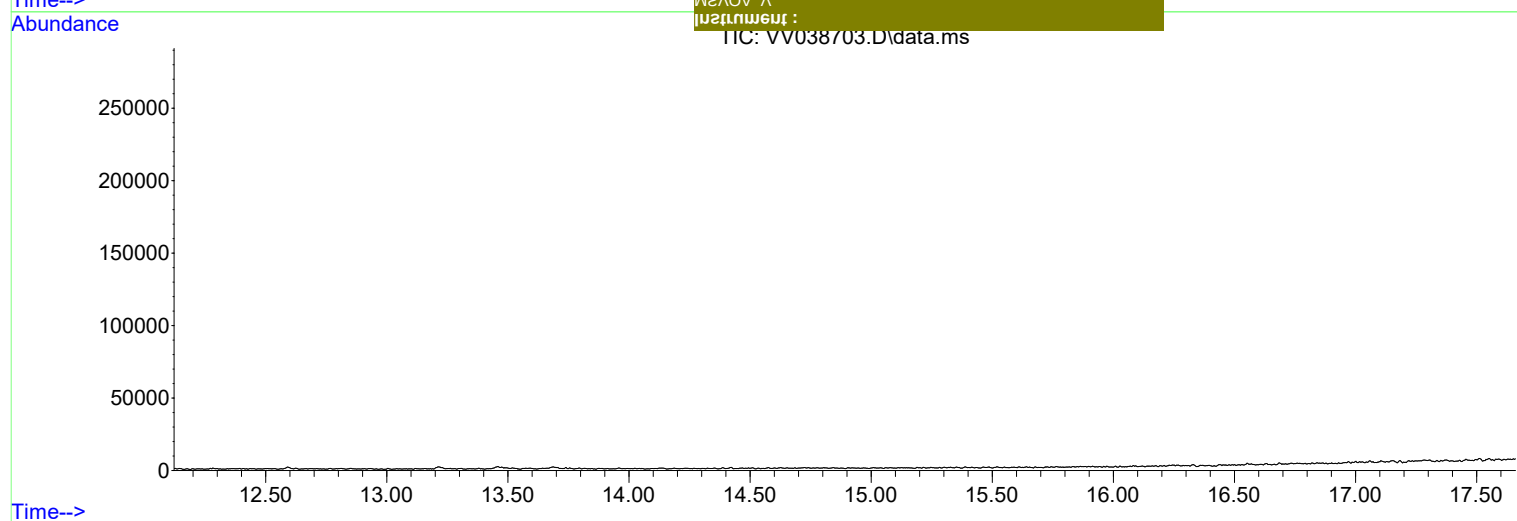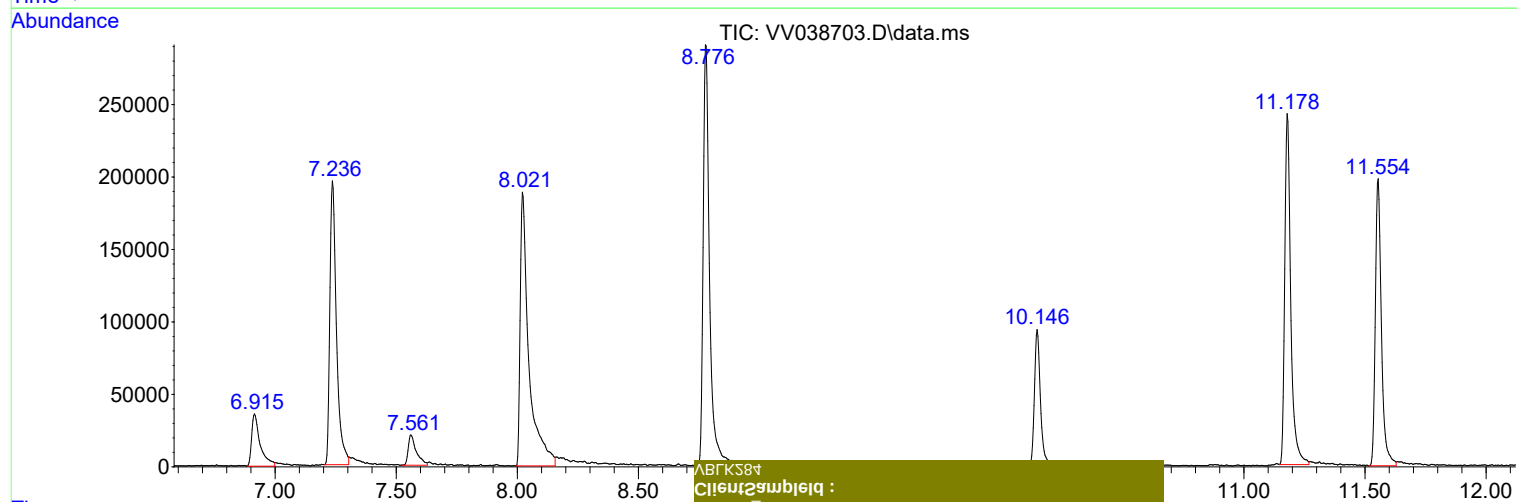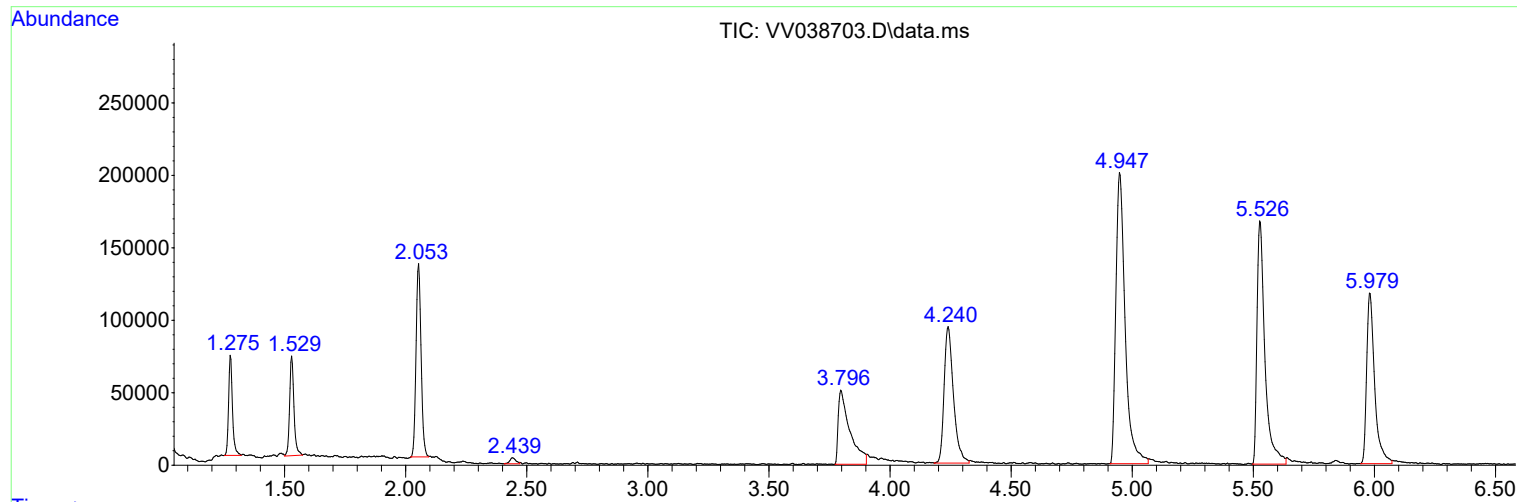

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV031325\  
Data File : VV038703.D  
Acq On : 13 Mar 2025 14:59  
Operator : SY/MD  
Sample : VV0313WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 10 Sample Multiplier: 1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR031325WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

LABK584  
Client Sampled :  
MSVOA\_V  
Instrument :

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV031325\  
Data File : VV038703.D  
Acq On : 13 Mar 2025 14:59  
Operator : SY/MD  
Sample : VV0313WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 10 Sample Multiplier: 1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR031325WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |    |      |      |
|------------------|----|---------|-------|----------|-------------------------|----|------|------|
|                  |    |         |       |          | #                       | RT | Resp | Conc |

VBTKS84  
Client Sample :  
MSVOA\_V  
Instrument :