

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031419\
 Data File : VV009672.D
 Acq On : 14 Mar 2019 18:05
 Operator : SY/MD
 Sample : K1885-09
 Misc : 5.95G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF193

Quant Time: Mar 15 05:37:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 04:30:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	89644	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85918	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	33842	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	28256	24.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.60%
7) Chloroethane-d5	1.57	69	27925	19.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.00%
10) 1,1-Dichloroethene-d2	2.13	63	57662	18.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.44%
20) 2-Butanone-d5	3.94	46	15917	53.01	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.02%
24) Chloroform-d	4.40	84	52214	22.85	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.40%
26) 1,2-Dichloroethane-d4	5.08	65	34478	26.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.64%
29) Benzene-d6	5.10	84	116471	25.84	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.36%
33) 1,2-Dichloropropane-d6	6.12	67	34531	26.22	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.88%
37) Toluene-d8	7.36	98	108116	24.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.16%
38) trans-1,3-Dichloropropene-	7.67	79	12933	21.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.48%
39) 2-Hexanone-d5	8.13	63	10804	44.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.10%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	30160	24.19	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.76%
61) 1,2-Dichlorobenzene-d4	11.68	152	33170	25.30	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	5168	3.960 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031419\
Data File : VV009672.D
Acq On : 14 Mar 2019 18:05
Operator : SY/MD
Sample : K1885-09
Misc : 5.95G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF193

Quant Time: Mar 15 05:37:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 04:30:02 2019
Response via : Initial Calibration

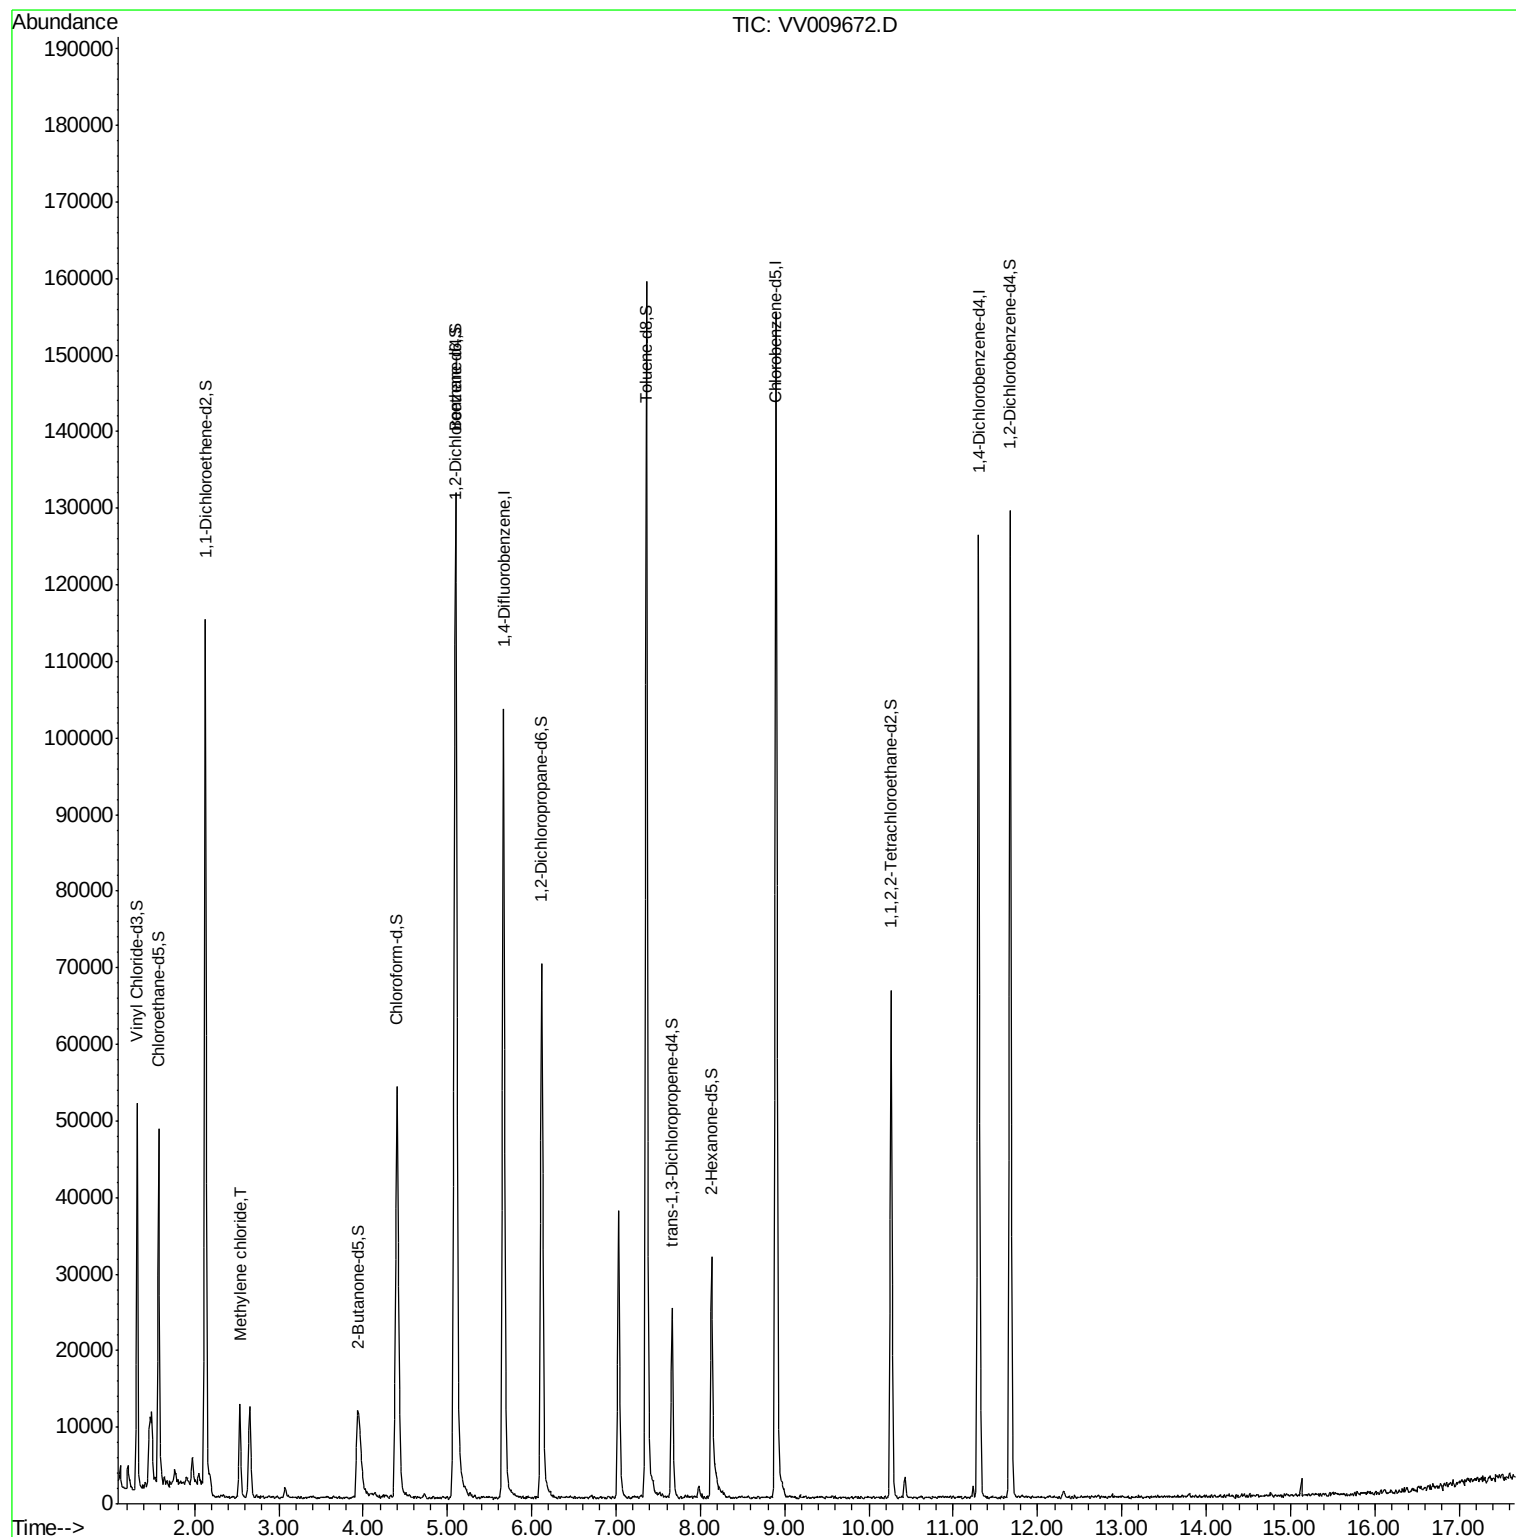

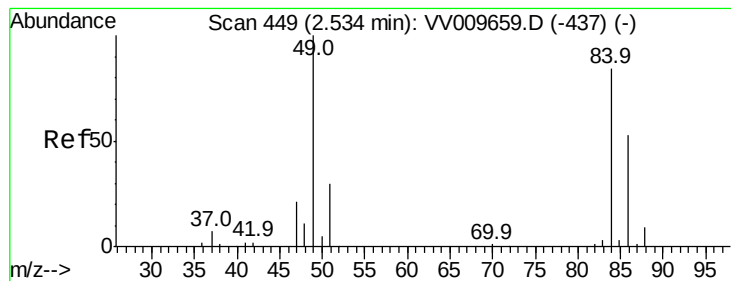

#16
 Methvlene chloride
 Concen: 3.960 ug/L
 RT: 2.54 min Scan# 450
 Delta R.T. 0.00 min
 Lab File: VV009672.D
 Acq: 14 Mar 2019 18:05

Instrument :
 MSVOA_V
 ClientSampleId :
 BF193

Tot Ion: 84 Resp: 5168
 Ion Ratio Lower Upper
 84 100
 49 107.8 86.1 159.9
 86 61.6 45.2 84.0

