


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031419\
Data File : VV009658.D
Acq On : 14 Mar 2019 09:24
Operator : SY/MD
Sample : BFB76
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB76

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
Title : VOC Analysis
Last Update : Fri Mar 15 04:30:02 2019

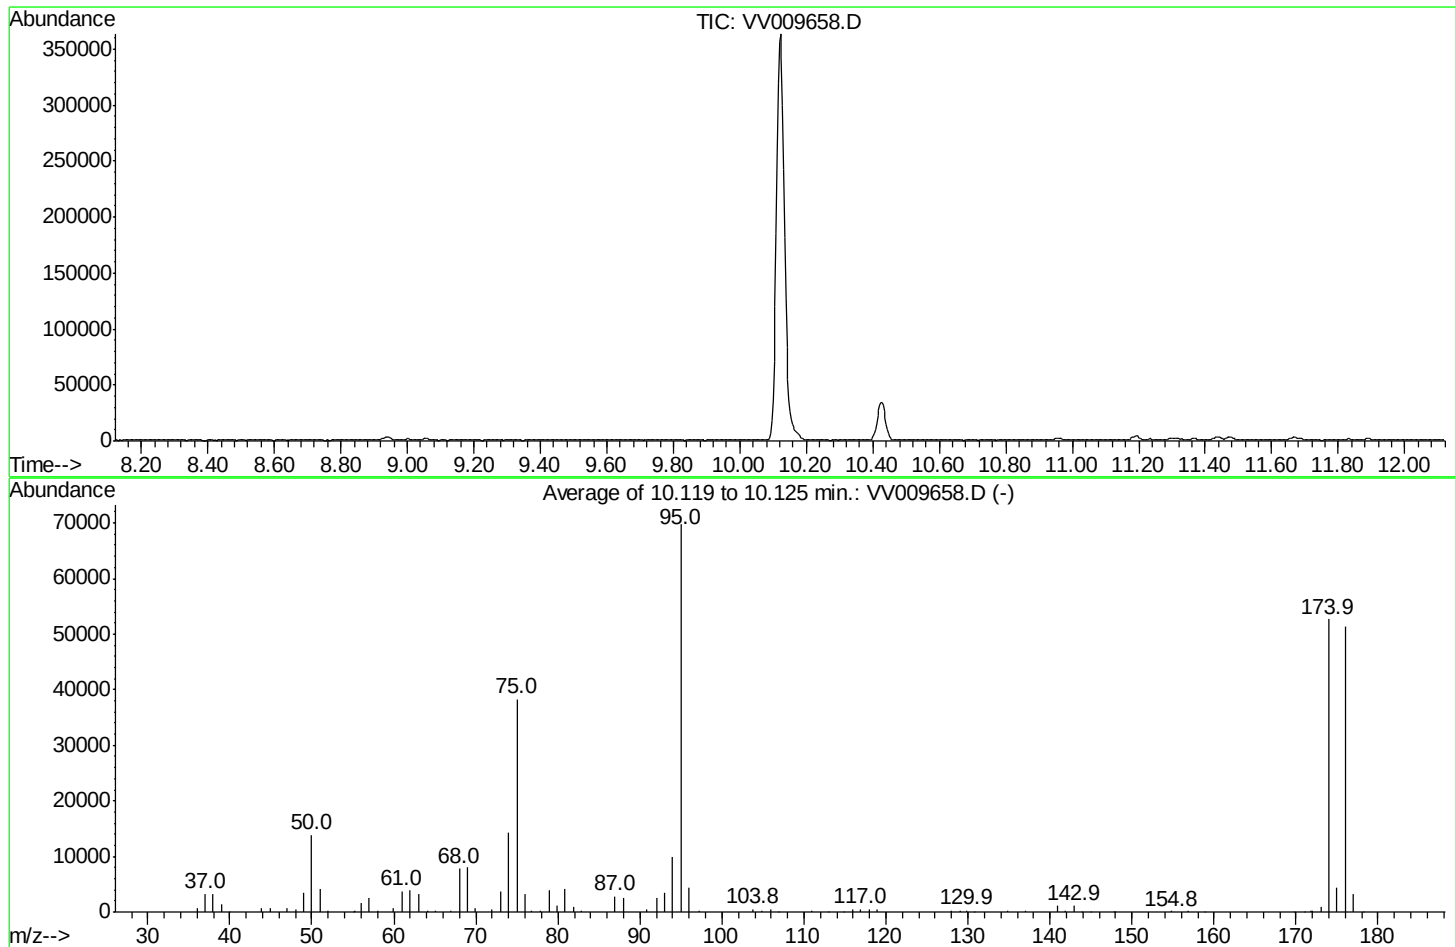

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	13851	PASS
75	95	30	80	54.9	38288	PASS
95	95	100	100	100.0	69752	PASS
96	95	5	9	6.4	4448	PASS
173	174	0.00	2	1.8	939	PASS
174	95	50	120	75.5	52653	PASS
175	174	5	9	8.5	4499	PASS
176	174	95	101	97.7	51458	PASS
177	176	5	9	6.2	3170	PASS

Scan 2796 (10.080 min): VV009658.D
BFB76

m/z	Abundance
39.90	600.0
43.80	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.00	819.0
37.00	3585.0
38.00	3401.0
39.00	1448.0
39.90	631.0
43.90	718.0
45.00	755.0
46.90	736.0
48.00	492.0
49.00	3600.0
50.00	14499.0
51.00	4154.0
52.00	234.0
55.00	184.0
56.00	1715.0
56.90	2443.0
58.10	146.0
60.00	809.0
61.00	3895.0
62.00	4125.0
63.00	3301.0
64.10	267.0
65.10	182.0
66.90	258.0
68.00	7973.0
69.00	8367.0
69.90	801.0
71.90	403.0
73.00	3669.0
74.00	14530.0
75.00	38816.0
76.00	3353.0
76.80	440.0
77.90	220.0
78.90	4130.0
79.90	1220.0
80.90	4205.0
81.90	1033.0
82.90	152.0
86.90	2867.0
87.90	2429.0
90.80	423.0
92.00	2522.0
93.00	3399.0
94.00	9727.0
95.00	70080.0
96.00	4672.0
97.20	141.0
103.80	561.0
104.90	184.0
105.90	453.0
106.90	122.0
110.90	137.0
115.90	356.0
117.00	520.0
117.90	372.0
118.90	516.0
127.90	281.0
129.00	178.0
129.90	335.0
130.70	138.0
134.70	209.0
137.00	199.0
140.90	1140.0
141.90	145.0
143.00	1200.0
144.80	110.0
147.70	164.0
154.80	177.0
156.80	110.0
158.90	107.0
171.80	511.0
173.00	921.0
174.00	51720.0
175.00	4338.0
176.00	50616.0
177.00	3186.0
178.20	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.00	717.0
37.00	3314.0
37.90	3329.0
39.00	1436.0
39.90	609.0
44.00	826.0
45.00	721.0
46.90	648.0
48.00	481.0
49.00	3589.0
50.00	14229.0
51.00	4154.0
52.00	222.0
55.20	214.0
56.00	1692.0
57.00	2557.0
58.10	149.0
59.90	709.0
61.00	3827.0
62.00	4009.0
63.00	3297.0
64.10	298.0
65.10	170.0
66.90	251.0
68.00	8026.0
69.00	8331.0
70.00	827.0
71.90	393.0
73.00	3725.0
74.00	14604.0
75.00	39080.0
76.00	3407.0
77.90	303.0
78.90	4067.0
79.90	1269.0
80.90	4211.0
81.90	989.0
82.90	125.0
87.00	2849.0
88.00	2606.0
90.80	399.0
92.00	2518.0
93.00	3447.0
94.00	10133.0
95.00	71792.0
96.00	4547.0
97.10	168.0
103.80	541.0
104.80	156.0
105.90	472.0
106.90	127.0
110.90	131.0
112.90	112.0
116.00	394.0
117.00	595.0
117.90	378.0
119.00	519.0
127.90	255.0
129.10	187.0
129.90	361.0
130.70	127.0
134.80	185.0
136.90	176.0
140.90	1188.0
141.90	139.0
143.00	1181.0
144.90	106.0
147.90	169.0
154.80	176.0
156.90	151.0
169.80	110.0
172.00	498.0
173.00	974.0
173.90	54048.0
175.00	4641.0
176.00	52856.0
177.00	3228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.10	583.0
37.00	2940.0
37.90	3036.0
39.00	1332.0
39.90	600.0
44.00	845.0
45.00	565.0
46.90	601.0
48.00	503.0
49.00	3163.0
50.00	12827.0
51.00	3902.0
52.00	198.0
55.20	223.0
56.00	1465.0
56.90	2443.0
58.10	120.0
59.90	633.0
61.00	3436.0
62.00	3597.0
63.00	3098.0
64.00	300.0
65.00	198.0
66.90	228.0
68.00	7375.0
69.00	7491.0
70.00	807.0
71.80	372.0
73.00	3610.0
74.00	13587.0
75.00	36968.0
76.00	3197.0
76.80	392.0
77.90	341.0
78.90	3891.0
79.90	1241.0
80.90	3941.0
81.90	883.0
82.90	114.0
87.00	2655.0
88.00	2593.0
90.80	330.0
92.00	2425.0
93.00	3231.0
94.00	9607.0
95.00	67384.0
96.00	4125.0
97.10	163.0
103.80	484.0
104.80	139.0
105.90	449.0
106.90	109.0
110.90	118.0
112.90	121.0
114.80	111.0
116.00	344.0
116.90	575.0
117.90	384.0
119.00	462.0
127.90	245.0
129.00	197.0
129.90	335.0
130.70	101.0
134.80	189.0
136.90	141.0
140.90	1066.0
141.90	123.0
142.90	1042.0
143.90	101.0
145.00	125.0
148.00	183.0
154.90	169.0
156.90	175.0
169.80	112.0
171.10	128.0
172.00	513.0
173.00	922.0
174.00	52192.0
175.00	4520.0
175.90	50904.0
177.00	3097.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76