

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031423\
 Data File : VW030195.D
 Acq On : 14 Mar 2023 15:12
 Operator : SY/MD
 Sample : 01906-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM93

Quant Time: Mar 15 01:39:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 15 01:37:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	157215	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	155719	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	80134	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	53697	5.279	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.600%
7) Chloroethane-d5	1.539	69	46325	4.851	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	2.066	63	78612	3.759	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.200%
20) 2-Butanone-d5	3.825	46	88061	46.953	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.900%
24) Chloroform-d	4.262	84	99924	4.809	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
26) 1,2-Dichloroethane-d4	4.957	65	43124	5.084	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	4.973	84	186669	4.455	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	5.998	67	58802	4.665	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.252	98	165096	4.157	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.200%
43) trans-1,3-Dichloroprop...	7.564	79	19967	4.630	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.600%
46) 2-Hexanone-d5	8.037	63	77127	43.227	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.460%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	42520	4.741	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	11.570	152	62611	4.618	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.400%
Target Compounds						
42) Toluene	7.329	91	17165	0.373	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030195.D
Acq On : 14 Mar 2023 15:12
Operator : SY/MD
Sample : 01906-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM93

Quant Time: Mar 15 01:39:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 15 01:37:04 2023
Response via : Initial Calibration

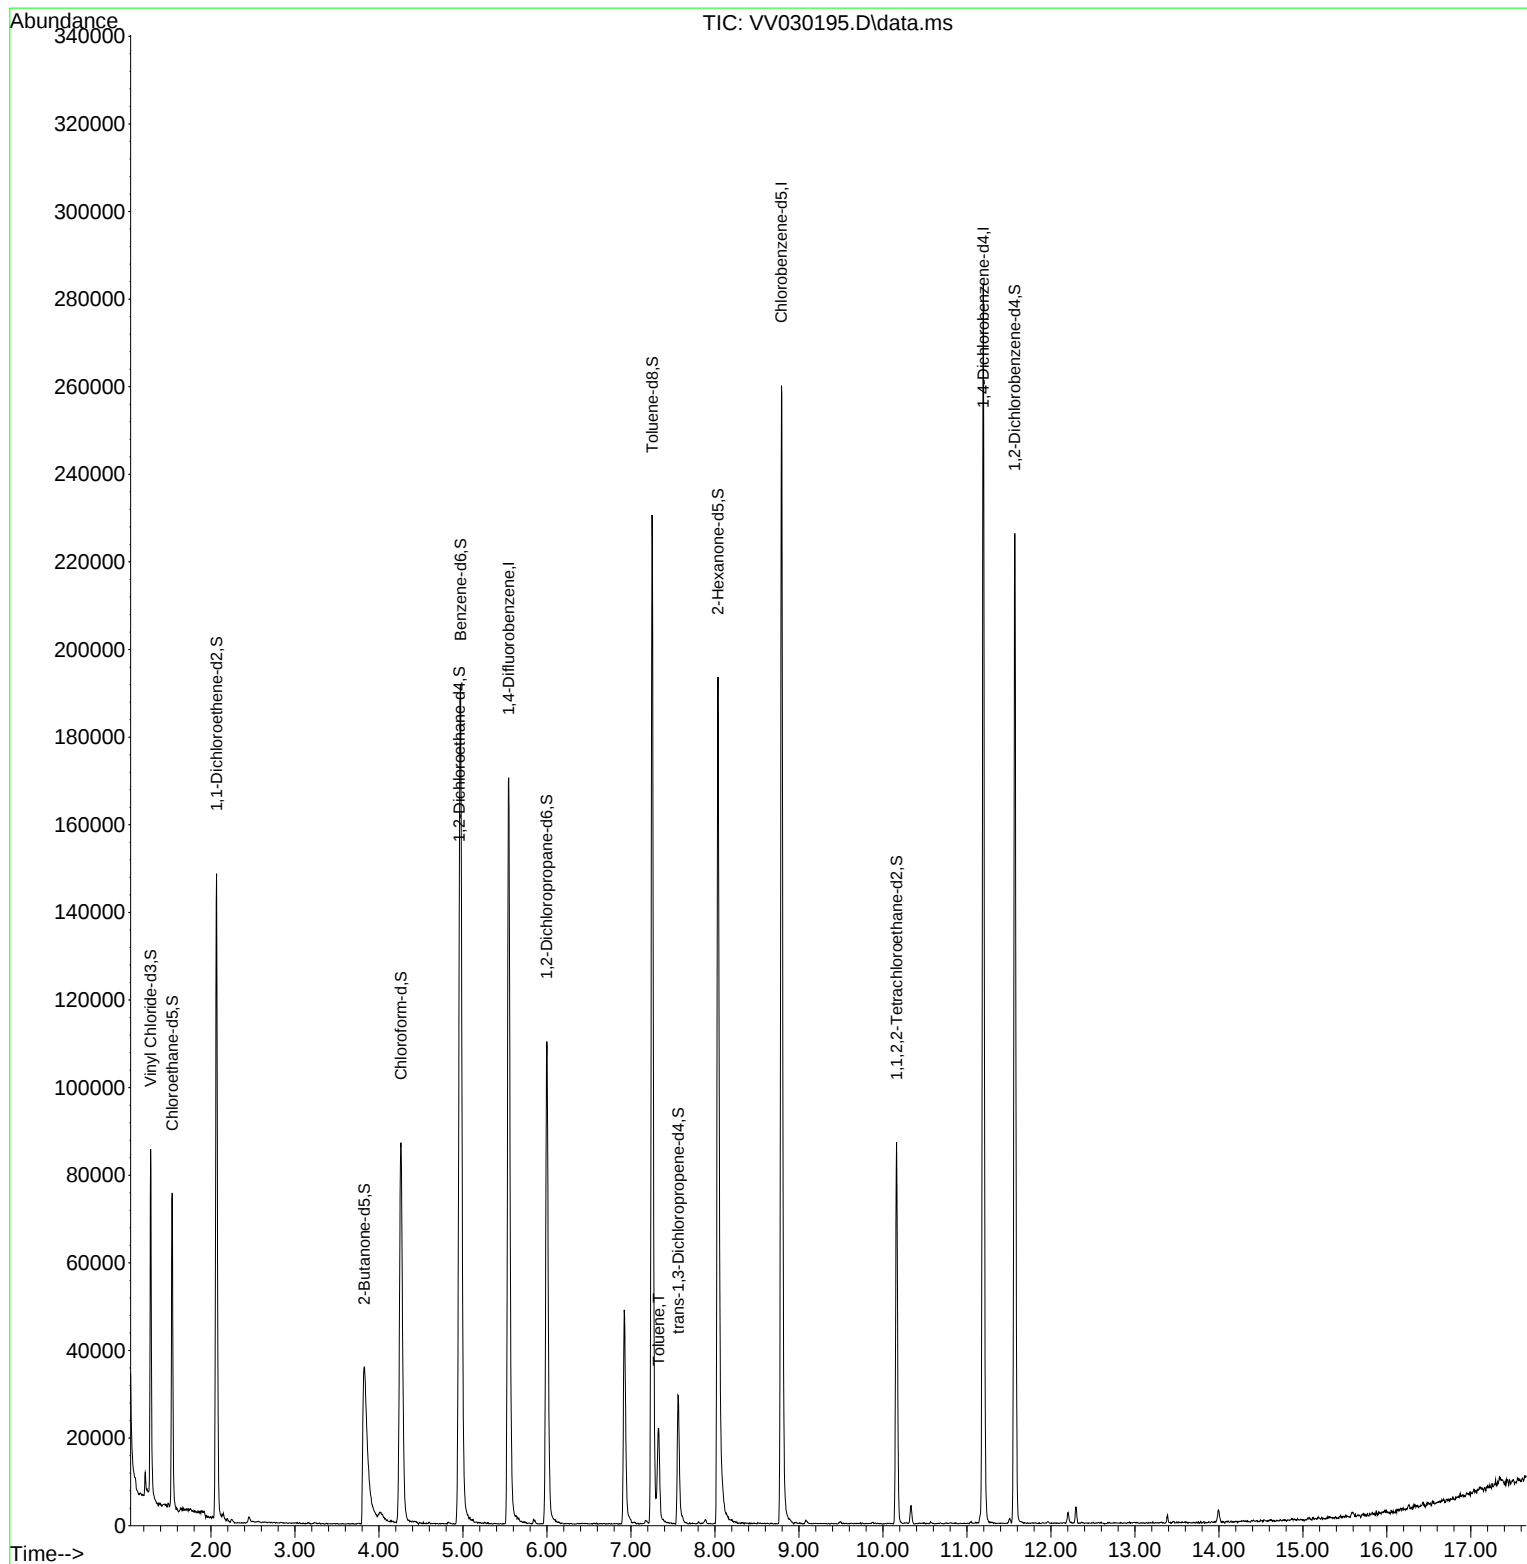

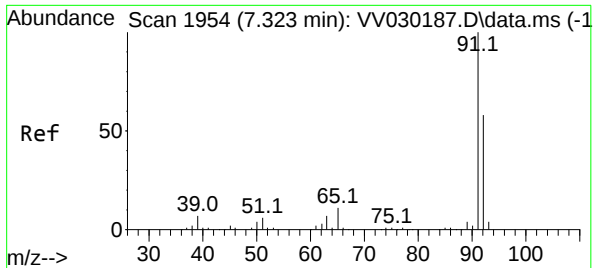

#42
Toluene
Concen: 0.373 ug/L
RT: 7.329 min Scan# 1956
Delta R.T. 0.006 min
Lab File: VV030195.D
Acq: 14 Mar 2023 15:12

Instrument :
MSVOA_V
ClientSampleId :
COM93

Tgt Ion: 91 Resp: 17165
Ion Ratio Lower Upper
91 100
92 55.7 39.6 73.6

