

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
 Data File : VV030197.D
 Acq On : 14 Mar 2023 16:00
 Operator : SY/MD
 Sample : 01906-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM95

Quant Time: Mar 15 01:40:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 15 01:37:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	152019	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	152891	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	76219	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	50468	5.131	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.600%
7) Chloroethane-d5	1.539	69	44774	4.849	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	2.066	63	74956	3.707	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.200%
20) 2-Butanone-d5	3.828	46	80946	44.634	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.260%
24) Chloroform-d	4.262	84	92061	4.582	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	4.953	65	40073	4.885	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%
32) Benzene-d6	4.973	84	177835	4.323	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
36) 1,2-Dichloropropane-d6	5.998	67	54805	4.428	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.600%
41) Toluene-d8	7.252	98	153320	3.932	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.600%
43) trans-1,3-Dichloroprop...	7.561	79	19522	4.610	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.200%
46) 2-Hexanone-d5	8.037	63	72007	41.104	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.200%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	40126	4.557	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.200%
66) 1,2-Dichlorobenzene-d4	11.571	152	58581	4.543	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.800%
Target Compounds						
					Qvalue	
13) Acetone	2.159	43	2817	2.102	ug/L	80
42) Toluene	7.330	91	9513	0.210	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030197.D
Acq On : 14 Mar 2023 16:00
Operator : SY/MD
Sample : 01906-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM95

Quant Time: Mar 15 01:40:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 15 01:37:04 2023
Response via : Initial Calibration

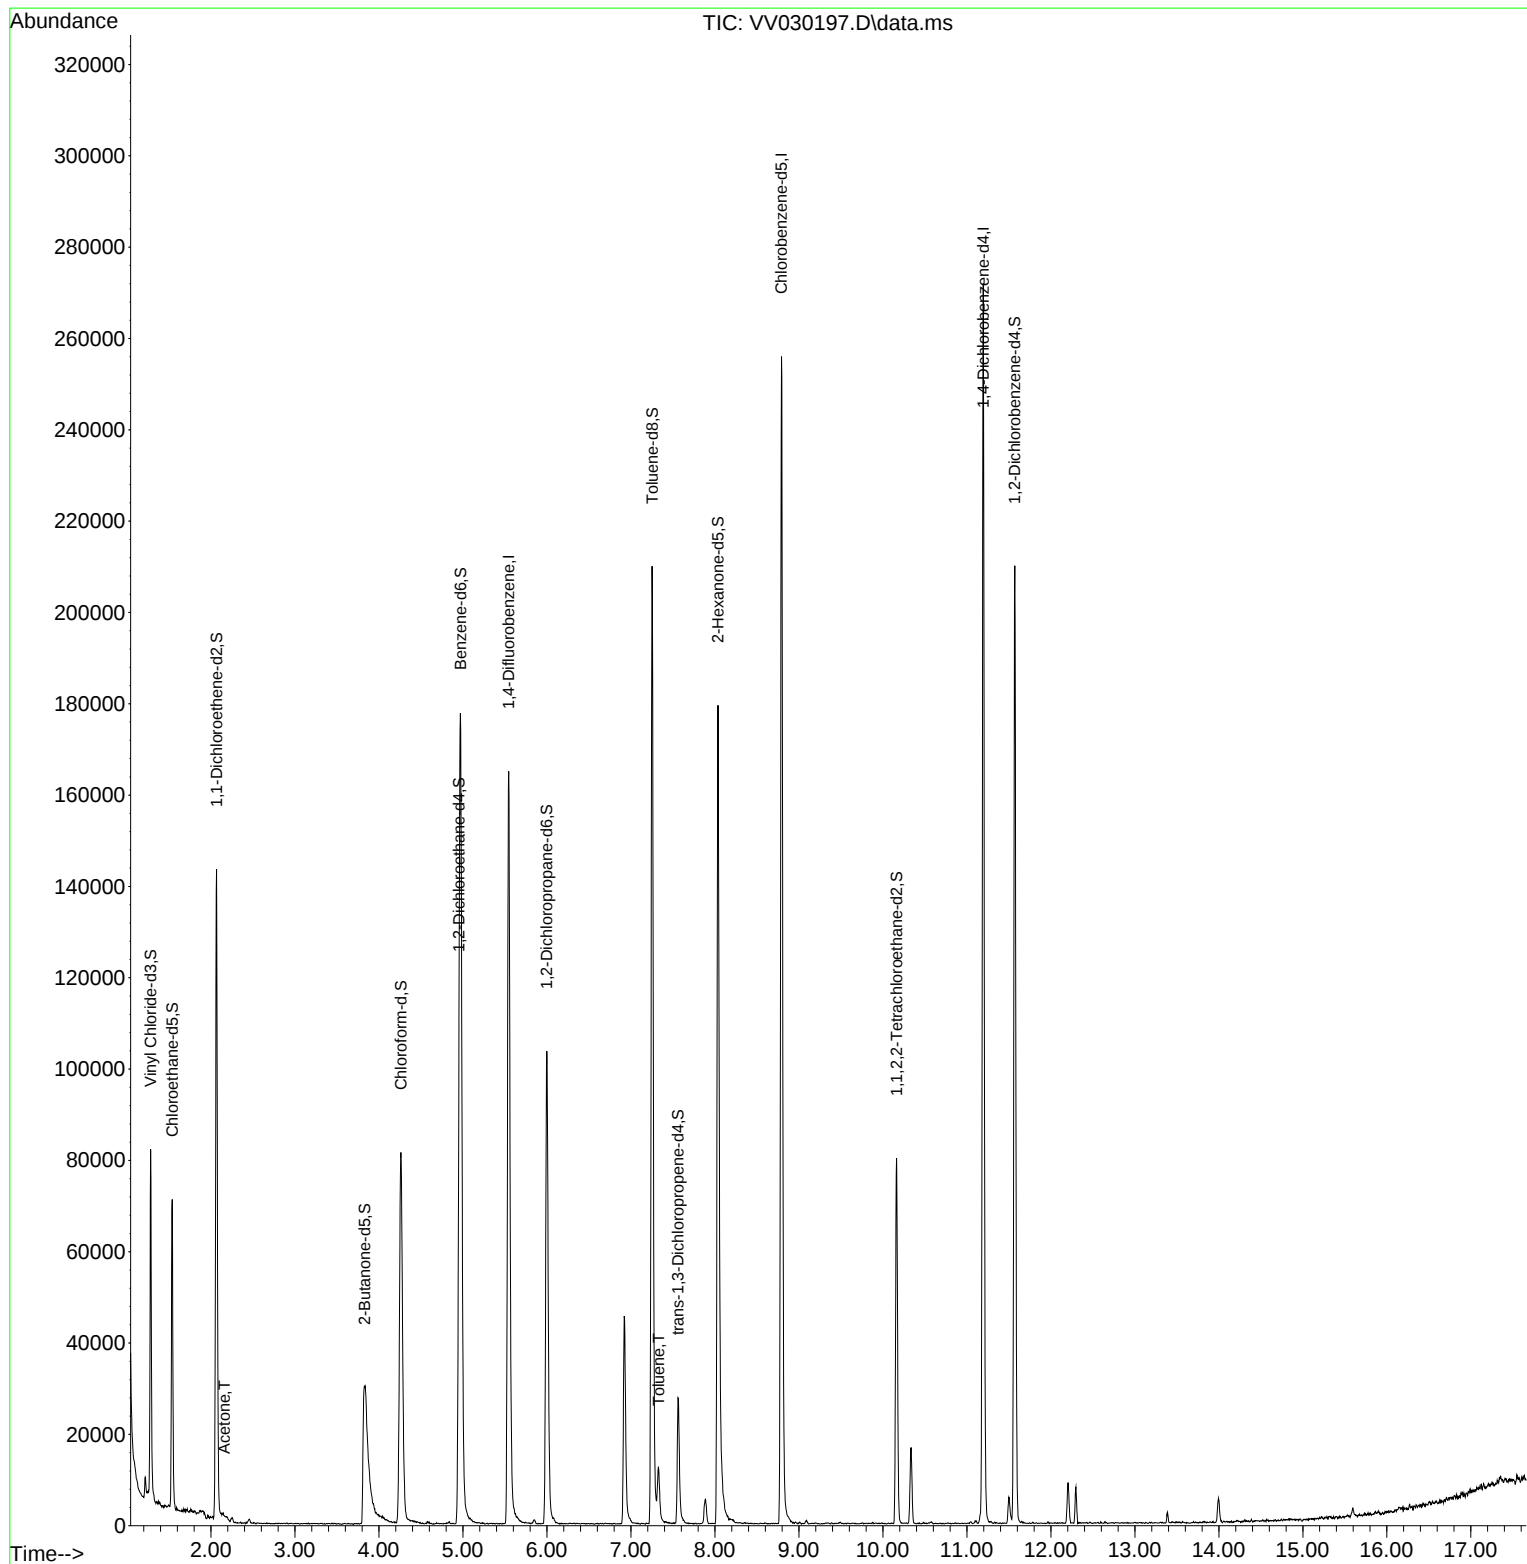

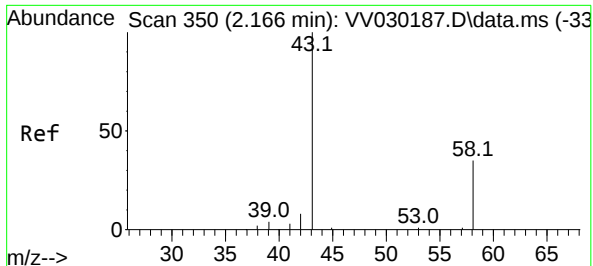

#13

Acetone

Concen: 2.102 ug/L

RT: 2.159 min Scan# 34

Delta R.T. -0.006 min

Lab File: VV030197.D

Acq: 14 Mar 2023 16:00

Instrument :

MSVOA_V

ClientSampleId :





COM95

Tgt Ion: 43 Resp: 2817

Ion Ratio Lower Upper

43 100

58 6.5 0.0 29.4

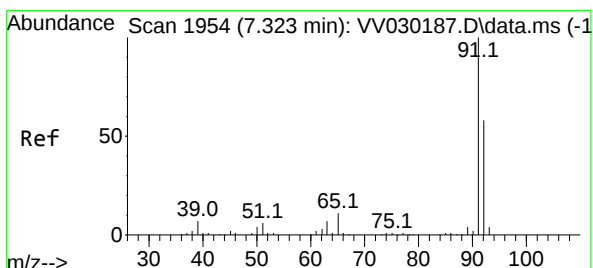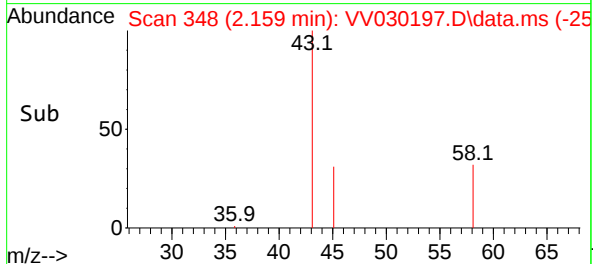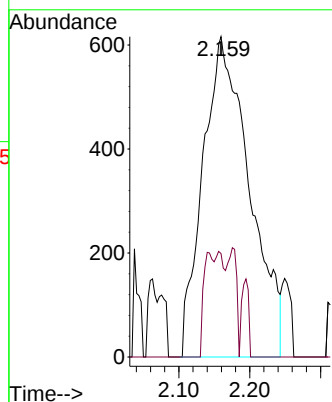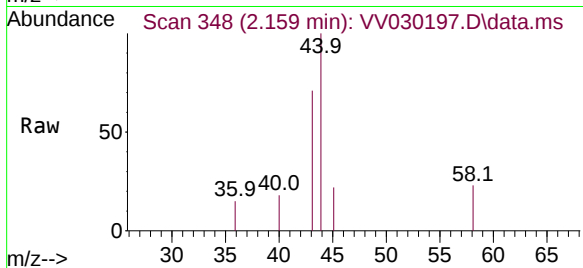

#42

Toluene

Concen: 0.210 ug/L

RT: 7.330 min Scan# 1956

Delta R.T. 0.006 min

Lab File: VV030197.D

Acq: 14 Mar 2023 16:00

Tgt Ion: 91 Resp: 9513

Ion Ratio Lower Upper

91 100

92 57.8 39.6 73.6

