

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
 Data File : VV030199.D
 Acq On : 14 Mar 2023 16:45
 Operator : SY/MD
 Sample : 01906-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM97

Quant Time: Mar 15 01:40:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 15 01:37:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	146382	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.796	117	144021	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	72444	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	47573	5.023	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.400%	
7) Chloroethane-d5	1.539	69	42131	4.739	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.800%	
11) 1,1-Dichloroethene-d2	2.066	63	68771	3.532	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	70.600%	
20) 2-Butanone-d5	3.825	46	74575	42.705	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	85.400%	
24) Chloroform-d	4.262	84	90419	4.673	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	4.957	65	39126	4.954	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.000%	
32) Benzene-d6	4.973	84	168209	4.341	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.800%	
36) 1,2-Dichloropropane-d6	6.002	67	52877	4.536	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.800%	
41) Toluene-d8	7.252	98	145890	3.972	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.400%	
43) trans-1,3-Dichloroprop...	7.564	79	18049	4.525	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.037	63	67511	40.911	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	81.820%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	39143	4.719	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.400%	
66) 1,2-Dichlorobenzene-d4	11.570	152	56710	4.627	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.600%	
Target Compounds						
42) Toluene	7.329	91	4296	0.101	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030199.D
Acq On : 14 Mar 2023 16:45
Operator : SY/MD
Sample : 01906-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM97

Quant Time: Mar 15 01:40:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 15 01:37:04 2023
Response via : Initial Calibration

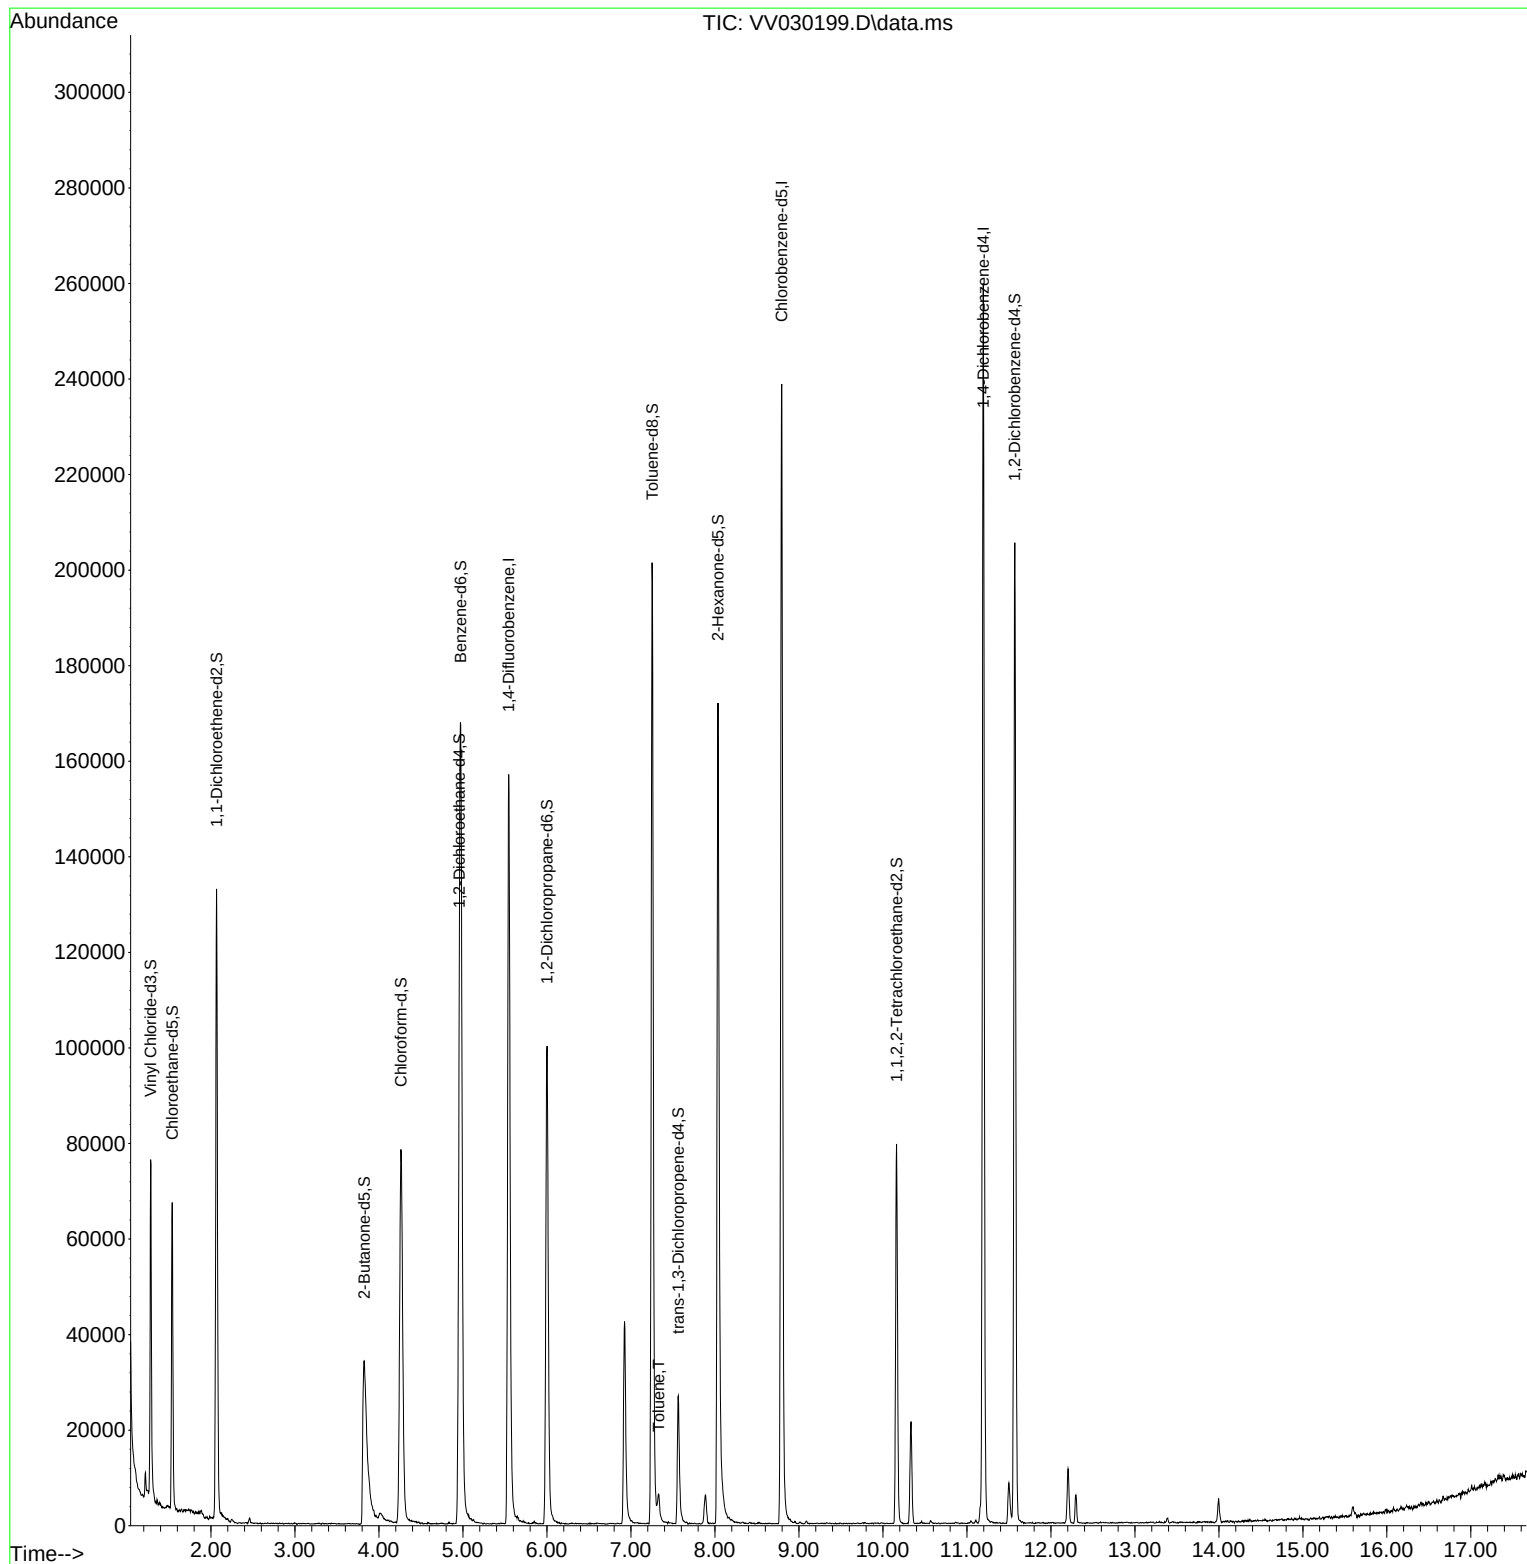

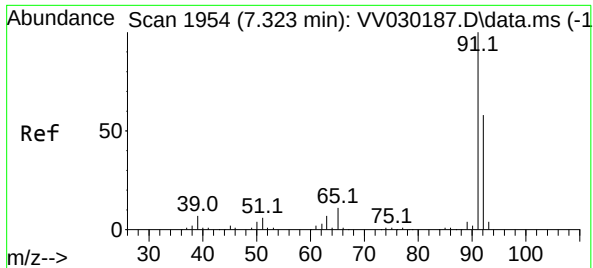

#42
Toluene
Concen: 0.101 ug/L
RT: 7.329 min Scan# 1954
Delta R.T. 0.006 min
Lab File: VV030199.D
Acq: 14 Mar 2023 16:45

Instrument :
MSVOA_V
ClientSampleId :
COM97

Tgt Ion: 91 Resp: 4296
Ion Ratio Lower Upper
91 100
92 55.5 39.6 73.6

