

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
 Data File : VV030188.D
 Acq On : 14 Mar 2023 11:46
 Operator : SY/MD
 Sample : VV0314WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK311

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	63	rBV	4557	4736	1.05%	0.126%
2	1.282	68	75	92	rVB	79378	87322	19.29%	2.327%
3	1.536	147	154	169	rVB	69841	81121	17.92%	2.162%
4	2.063	308	318	332	rBV	144245	210799	46.57%	5.619%
5	2.455	432	440	451	rVB2	4110	6616	1.46%	0.176%
6	3.854	860	875	915	rBV2	19066	112766	24.91%	3.006%
7	4.262	986	1002	1026	rBV	81432	206992	45.73%	5.517%
8	4.969	1205	1222	1259	rBV2	177002	452638	100.00%	12.065%
9	5.545	1388	1401	1421	rBV	147481	303894	67.14%	8.100%
10	5.998	1528	1542	1569	rBV	104788	219371	48.46%	5.847%
11	6.924	1815	1830	1849	rBV2	43819	84852	18.75%	2.262%
12	7.252	1920	1932	1957	rBV	203533	368373	81.38%	9.819%
13	7.564	2018	2029	2046	rBV	27225	49826	11.01%	1.328%
14	8.040	2166	2177	2222	rBV	158983	339708	75.05%	9.055%
15	8.792	2398	2411	2443	rBV	228415	384486	84.94%	10.248%
16	10.162	2825	2837	2856	rBV	81462	129721	28.66%	3.458%
17	11.194	3147	3158	3178	rBV	239897	370201	81.79%	9.867%
18	11.571	3263	3275	3292	rBV	207172	324878	71.77%	8.659%
19	12.204	3460	3472	3482	rBV3	5050	8662	1.91%	0.231%
20	13.995	4019	4029	4041	rBV2	2823	4816	1.06%	0.128%




Sum of corrected areas: 3751778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030188.D
Acq On : 14 Mar 2023 11:46
Operator : SY/MD
Sample : VV0314WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK311

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

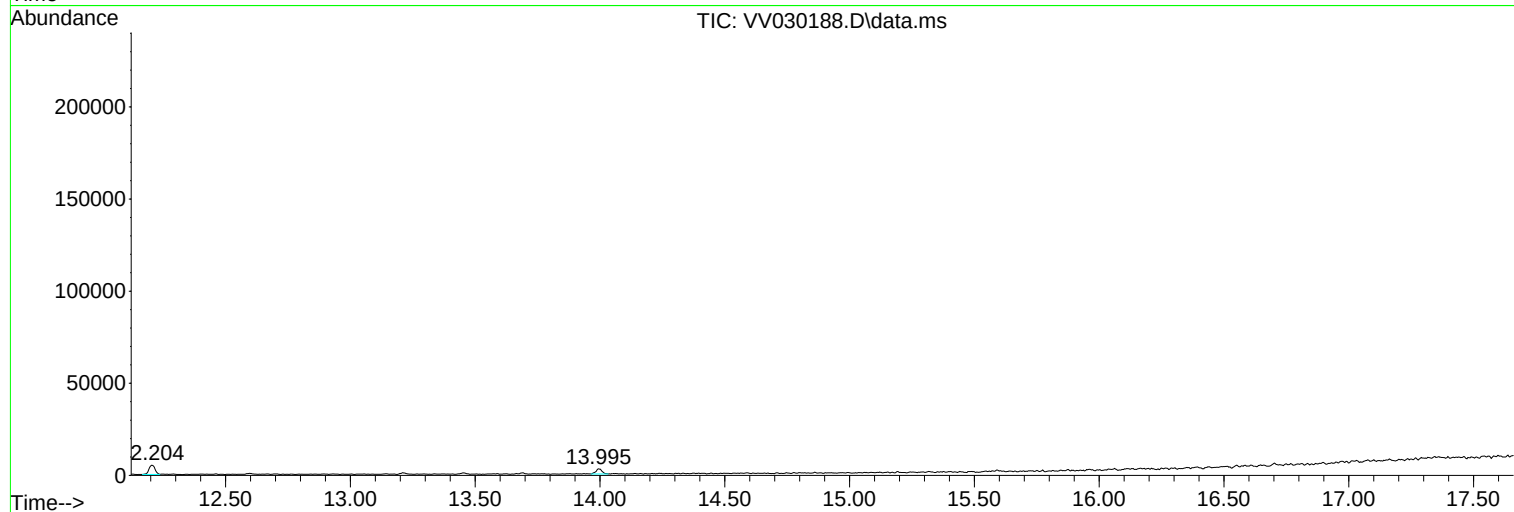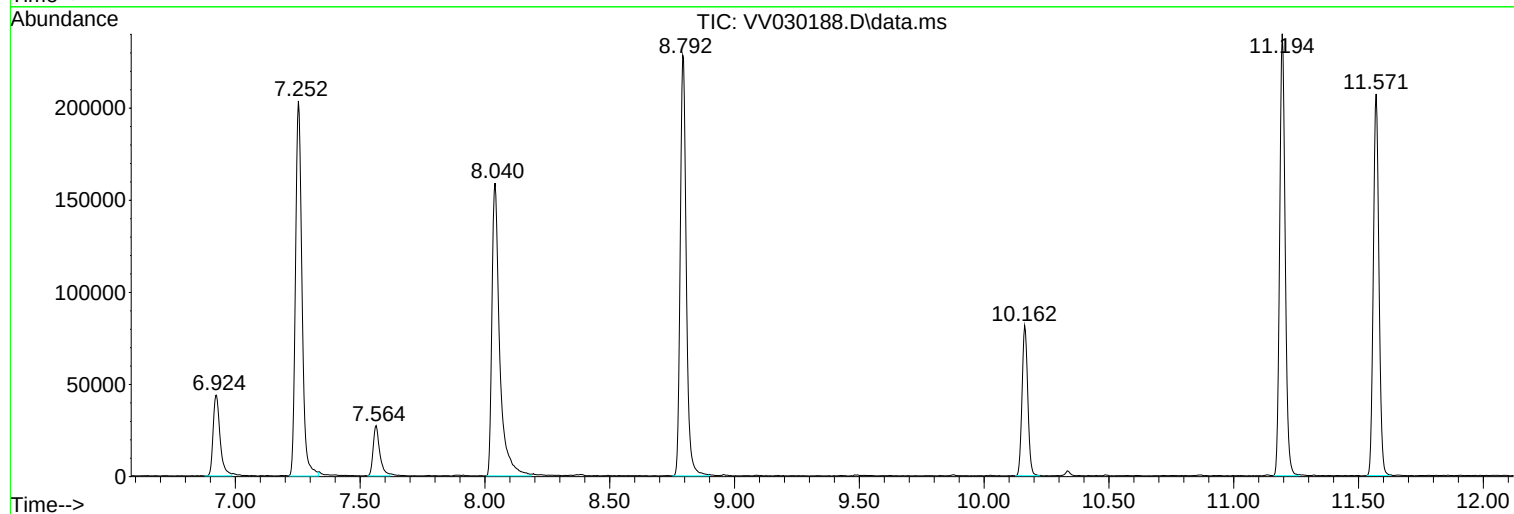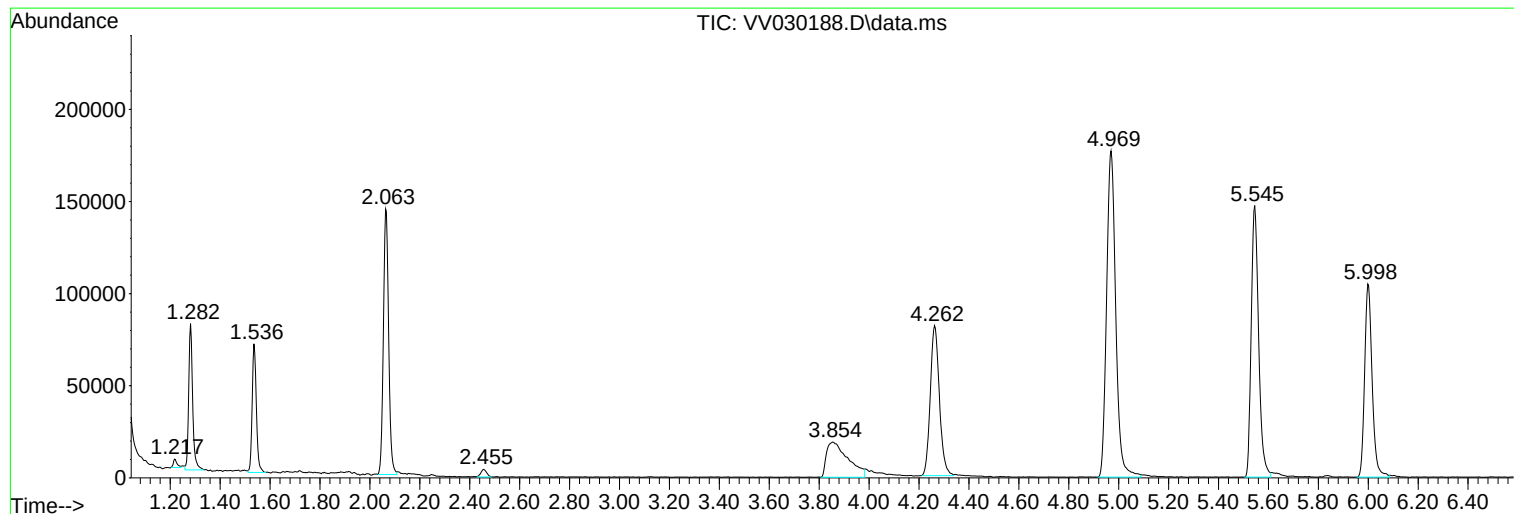

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030188.D
Acq On : 14 Mar 2023 11:46
Operator : SY/MD
Sample : VV0314WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK311

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030188.D
Acq On : 14 Mar 2023 11:46
Operator : SY/MD
Sample : VV0314WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK311

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc