

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
 Data File : VV030194.D
 Acq On : 14 Mar 2023 14:47
 Operator : SY/MD
 Sample : VIBLK278
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK278

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	64	rBV	3904	4800	1.00%	0.118%
2	1.281	69	75	97	rVB	79681	90896	18.95%	2.234%
3	1.539	147	155	168	rVB	70615	81252	16.94%	1.997%
4	2.066	309	319	335	rBV	145010	210047	43.78%	5.163%
5	2.458	433	441	450	rBV2	4543	6859	1.43%	0.169%
6	3.822	853	865	902	rBV2	37013	142050	29.61%	3.491%
7	4.262	985	1002	1032	rBV	83946	216255	45.08%	5.315%
8	4.969	1204	1222	1254	rBV2	188230	479730	100.00%	11.791%
9	5.545	1388	1401	1430	rBV	165976	346563	72.24%	8.518%
10	5.998	1526	1542	1566	rBV	108131	225169	46.94%	5.534%
11	6.924	1818	1830	1849	rBV	48750	90078	18.78%	2.214%
12	7.252	1920	1932	1967	rBV	225129	402559	83.91%	9.894%
13	7.561	2018	2028	2049	rBV	29260	53182	11.09%	1.307%
14	8.037	2165	2176	2218	rBV	192028	363772	75.83%	8.941%
15	8.792	2400	2411	2442	rBV	250699	426147	88.83%	10.474%
16	10.162	2826	2837	2854	rBV	82491	131369	27.38%	3.229%
17	10.336	2882	2891	2900	rVB2	4726	6983	1.46%	0.172%
18	11.194	3147	3158	3181	rBV	275837	425211	88.64%	10.451%
19	11.570	3263	3275	3293	rVV	227652	355048	74.01%	8.726%
20	12.204	3460	3472	3483	rBV2	7035	10721	2.23%	0.263%




Sum of corrected areas: 4068691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030194.D
Acq On : 14 Mar 2023 14:47
Operator : SY/MD
Sample : VIBLK278
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

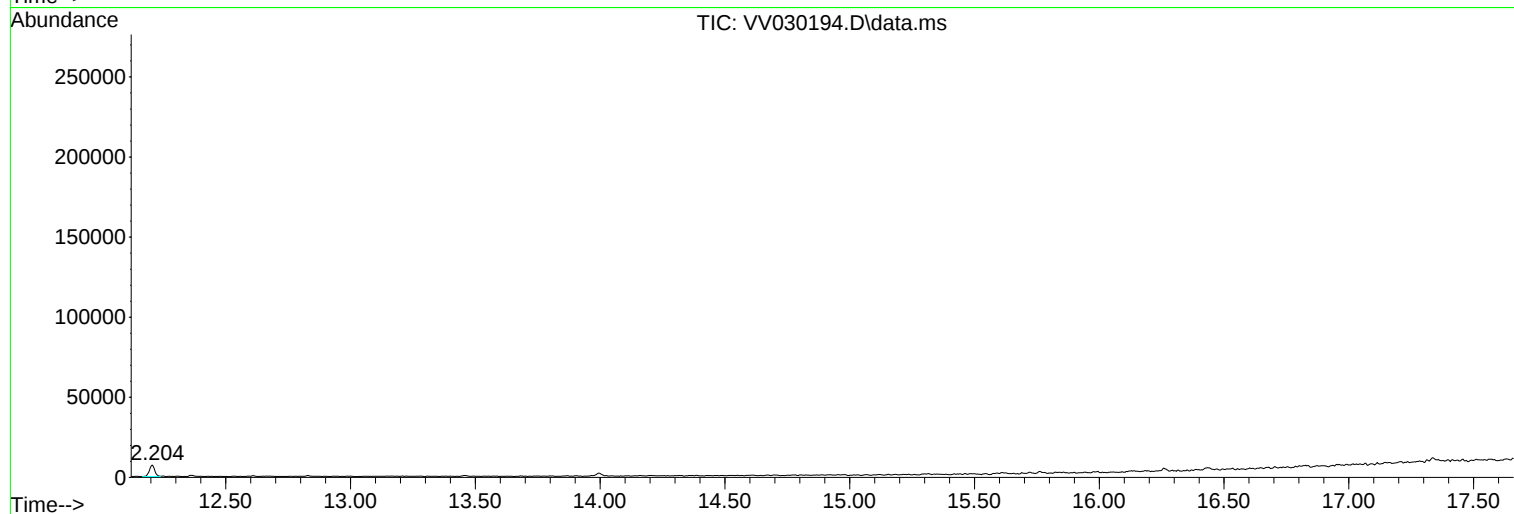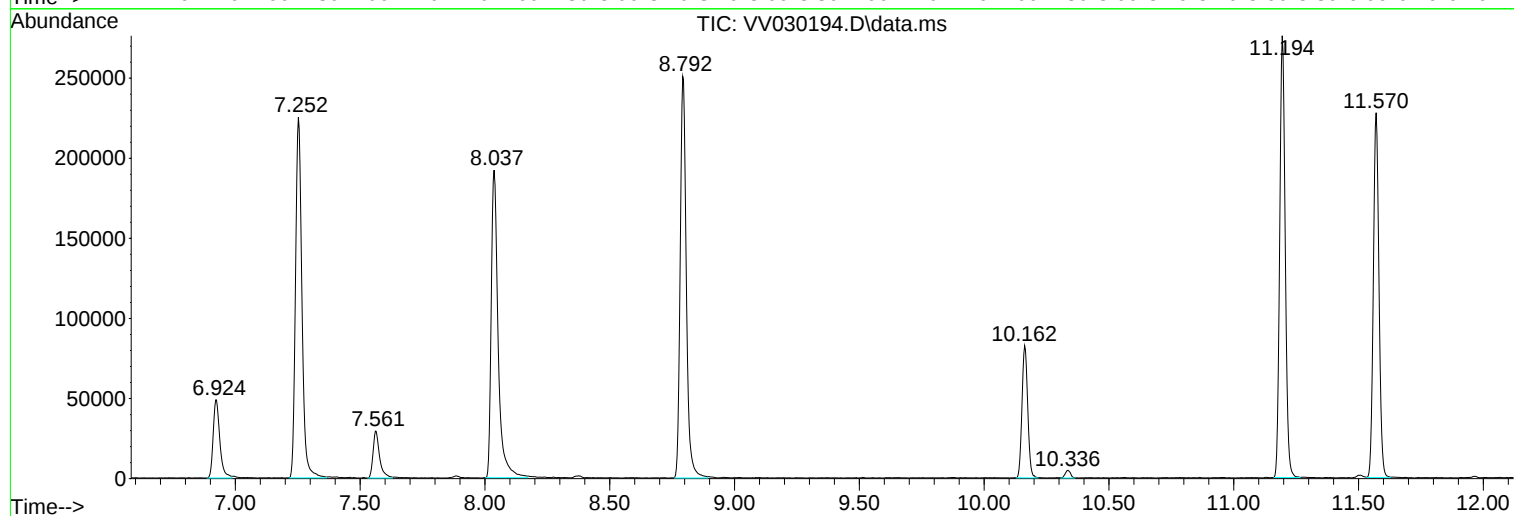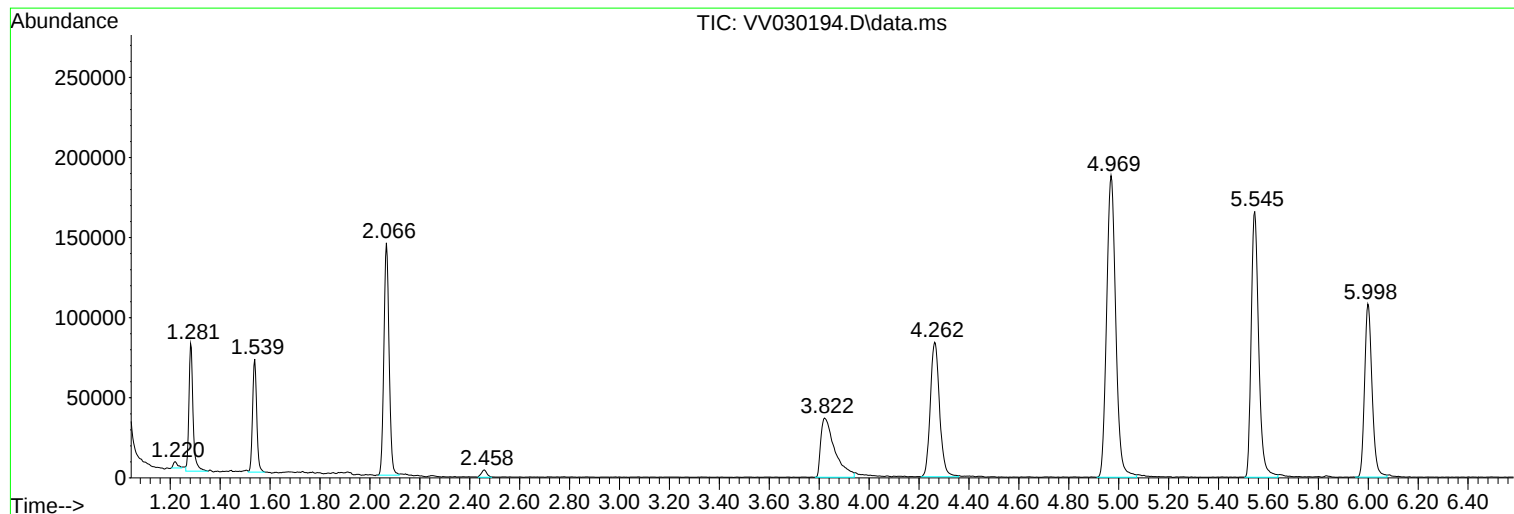

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030194.D
Acq On : 14 Mar 2023 14:47
Operator : SY/MD
Sample : VIBLK278
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030194.D
Acq On : 14 Mar 2023 14:47
Operator : SY/MD
Sample : VIBLK278
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc