

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
 Data File : VV030195.D
 Acq On : 14 Mar 2023 15:12
 Operator : SY/MD
 Sample : 01906-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM93

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	60	rBV	5262	5117	1.05%	0.122%
2	1.281	68	75	98	rVB	80866	93061	19.17%	2.219%
3	1.539	147	155	169	rVB	72167	85184	17.55%	2.031%
4	2.066	308	319	334	rBV	147059	215057	44.30%	5.128%
5	3.825	855	866	914	rBV2	35858	146594	30.19%	3.495%
6	4.262	985	1002	1027	rBV	86736	222609	45.85%	5.308%
7	4.969	1204	1222	1248	rBV2	191675	485507	100.00%	11.577%
8	5.545	1383	1401	1425	rBV	170343	355404	73.20%	8.474%
9	5.998	1526	1542	1569	rBV	110119	231566	47.70%	5.521%
10	6.921	1819	1829	1857	rBV	48843	93005	19.16%	2.218%
11	7.252	1920	1932	1946	rBV	230133	404079	83.23%	9.635%
12	7.326	1947	1955	1973	rVB	21010	41526	8.55%	0.990%
13	7.561	2019	2028	2055	rBV2	29397	55373	11.41%	1.320%
14	8.037	2165	2176	2214	rBV	193273	372096	76.64%	8.872%
15	8.792	2399	2411	2439	rBV	259733	437205	90.05%	10.425%
16	10.162	2826	2837	2853	rBV	87100	135992	28.01%	3.243%
17	10.336	2881	2891	2902	rVB	4209	6286	1.29%	0.150%
18	11.194	3141	3158	3179	rBV	282958	441811	91.00%	10.535%
19	11.570	3263	3275	3297	rBV	225895	356464	73.42%	8.500%
20	12.297	3494	3501	3511	rVB4	3751	4917	1.01%	0.117%
21	13.995	4019	4029	4040	rVB2	2880	5048	1.04%	0.120%




Sum of corrected areas: 4193901

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030195.D
Acq On : 14 Mar 2023 15:12
Operator : SY/MD
Sample : 01906-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

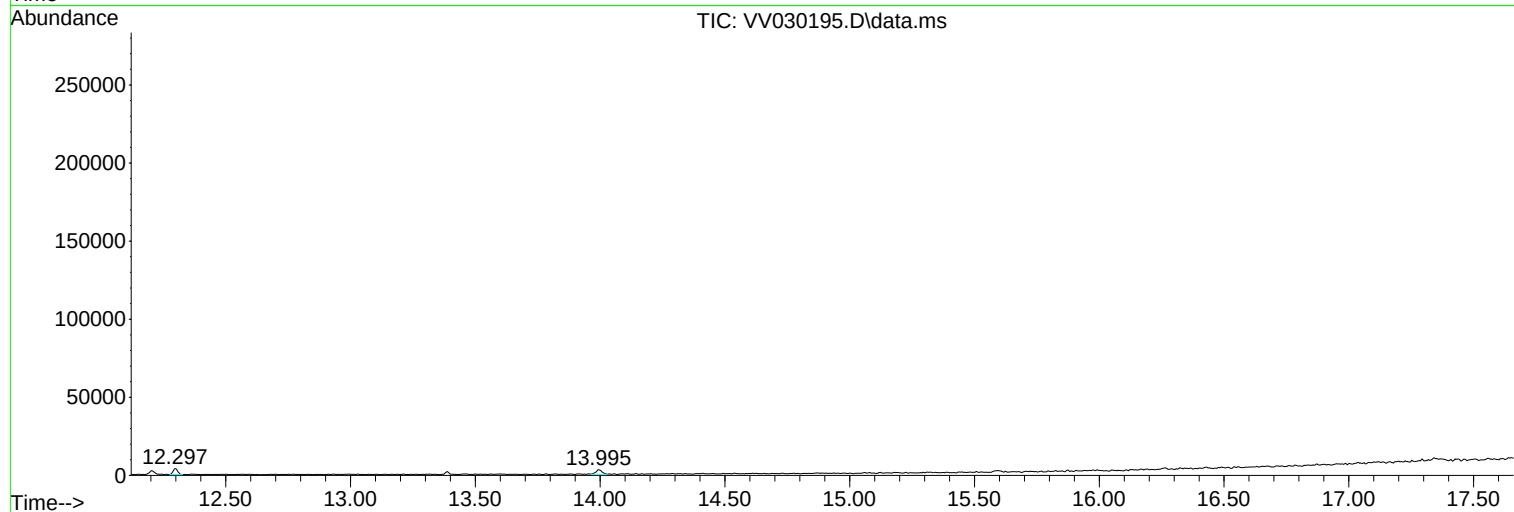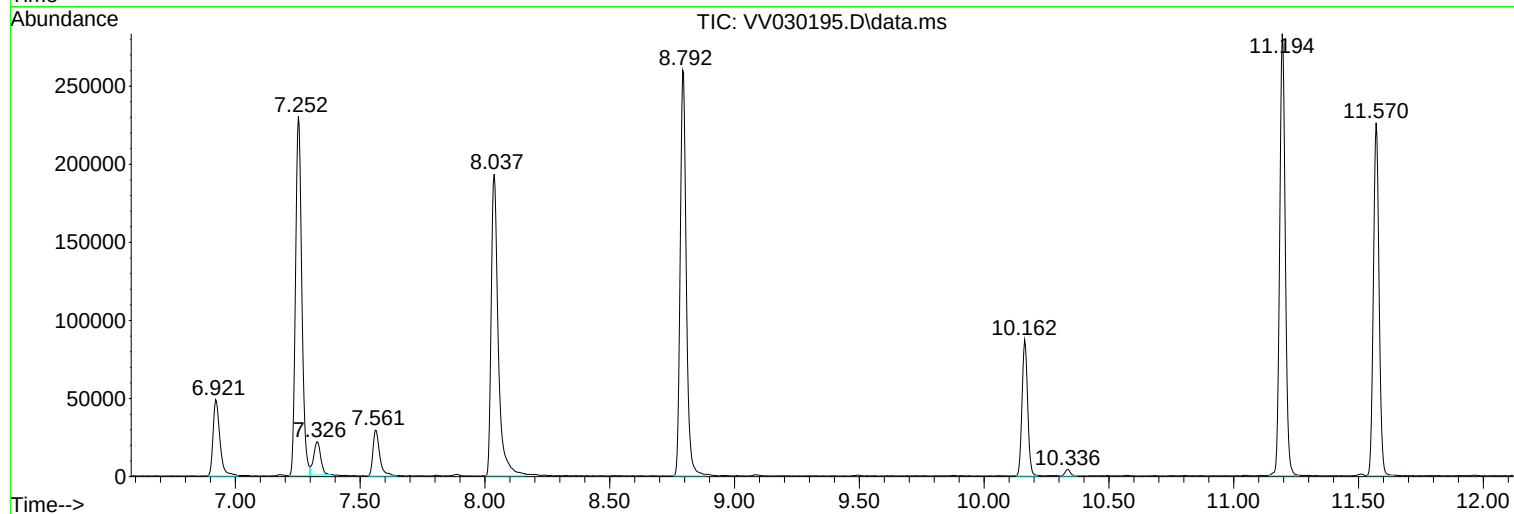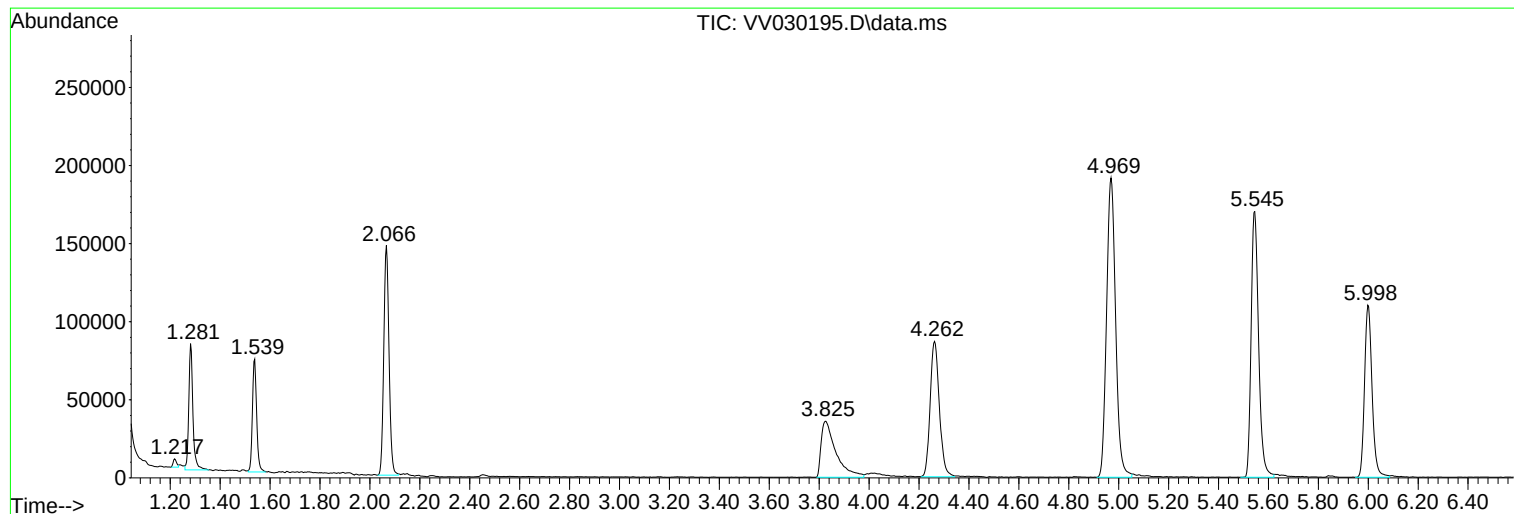

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030195.D
Acq On : 14 Mar 2023 15:12
Operator : SY/MD
Sample : 01906-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030195.D
Acq On : 14 Mar 2023 15:12
Operator : SY/MD
Sample : 01906-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc