

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
 Data File : VV030196.D
 Acq On : 14 Mar 2023 15:35
 Operator : SY/MD
 Sample : 01906-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM94

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	65	rBV2	4238	5925	1.22%	0.146%
2	1.282	68	75	93	rVB	80041	89285	18.39%	2.202%
3	1.539	147	155	169	rVB	72846	83753	17.25%	2.065%
4	2.066	307	319	332	rBV	146093	212862	43.85%	5.249%
5	3.831	855	868	899	rBV	30746	131482	27.09%	3.242%
6	4.262	984	1002	1026	rBV2	85369	219955	45.32%	5.424%
7	4.828	1168	1178	1190	rBV7	2334	5006	1.03%	0.123%
8	4.969	1200	1222	1252	rBV2	191630	485389	100.00%	11.969%
9	5.545	1388	1401	1430	rBV	155595	325568	67.07%	8.028%
10	5.998	1529	1542	1582	rBV2	111340	230495	47.49%	5.683%
11	6.921	1819	1829	1861	rBV	47289	90725	18.69%	2.237%
12	7.252	1919	1932	1947	rBV	227508	399112	82.23%	9.841%
13	7.326	1947	1955	1977	rVB	28335	55949	11.53%	1.380%
14	7.561	2017	2028	2057	rBV	30329	54352	11.20%	1.340%
15	8.037	2165	2176	2222	rBV2	182615	366044	75.41%	9.026%
16	8.792	2396	2411	2438	rBV	239007	402656	82.96%	9.929%
17	10.162	2825	2837	2851	rBV	84981	132079	27.21%	3.257%
18	10.336	2881	2891	2901	rBV2	5812	8726	1.80%	0.215%
19	11.194	3140	3158	3179	rBV	255076	391738	80.71%	9.659%
20	11.571	3263	3275	3290	rBV	221545	346914	71.47%	8.554%
21	12.207	3463	3473	3482	rBV2	3749	5568	1.15%	0.137%
22	12.297	3492	3501	3508	rBB5	4156	5298	1.09%	0.131%
23	13.998	4019	4030	4037	rBV	4055	6631	1.37%	0.164%




Sum of corrected areas: 4055512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030196.D
Acq On : 14 Mar 2023 15:35
Operator : SY/MD
Sample : 01906-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

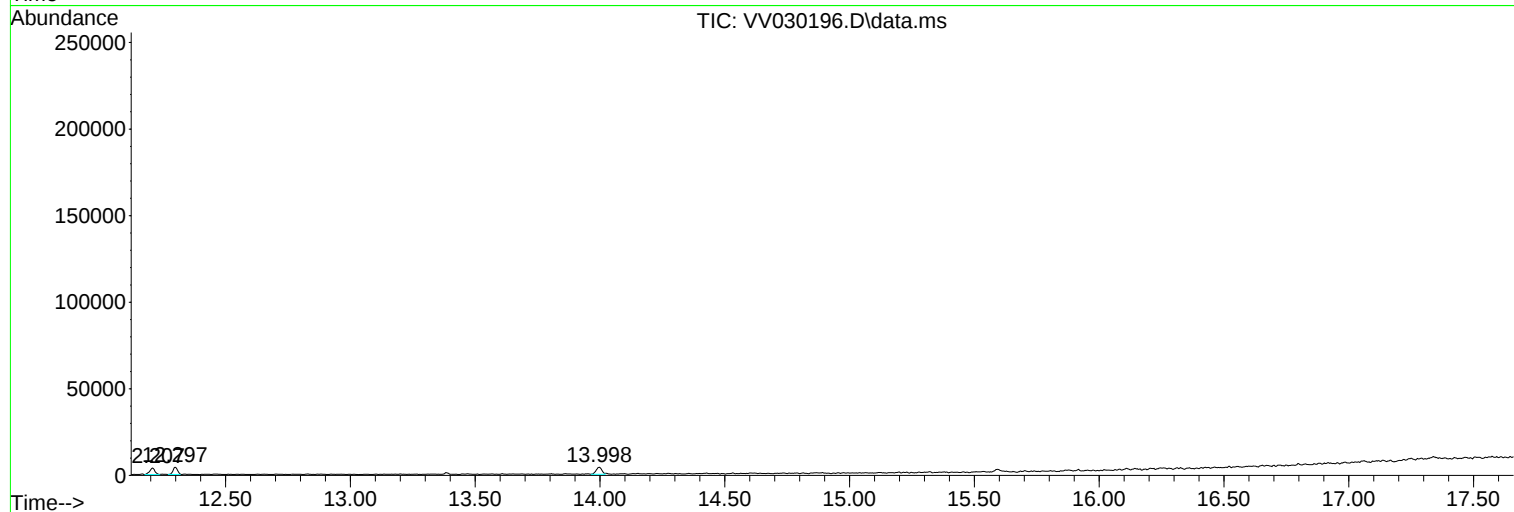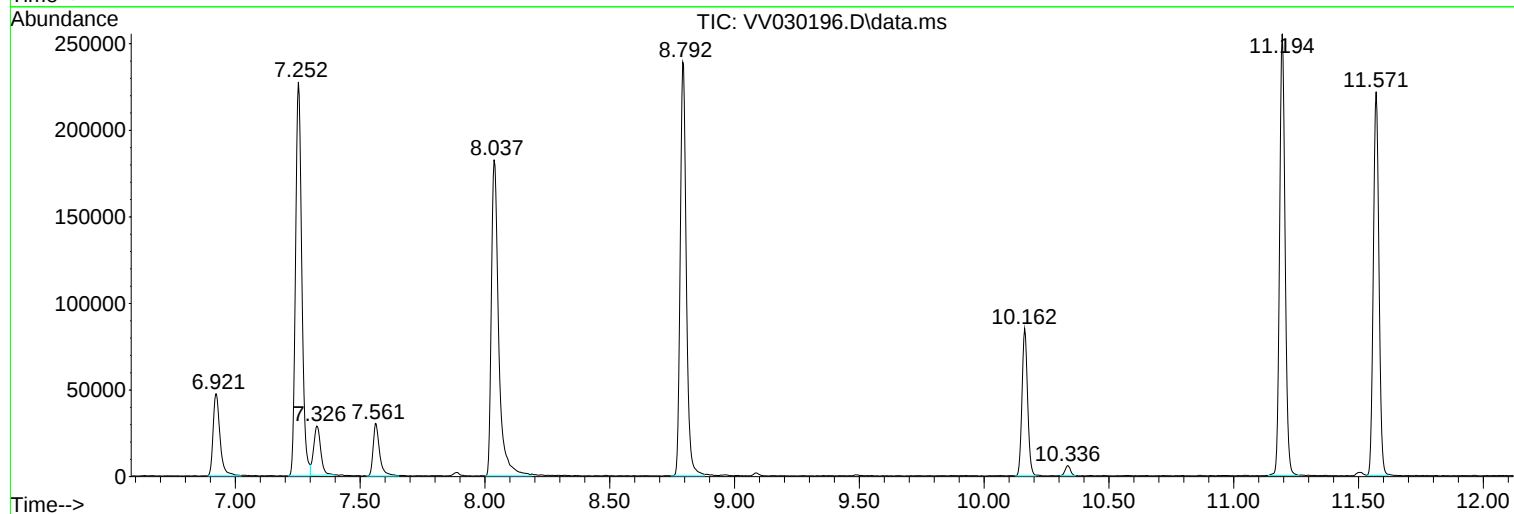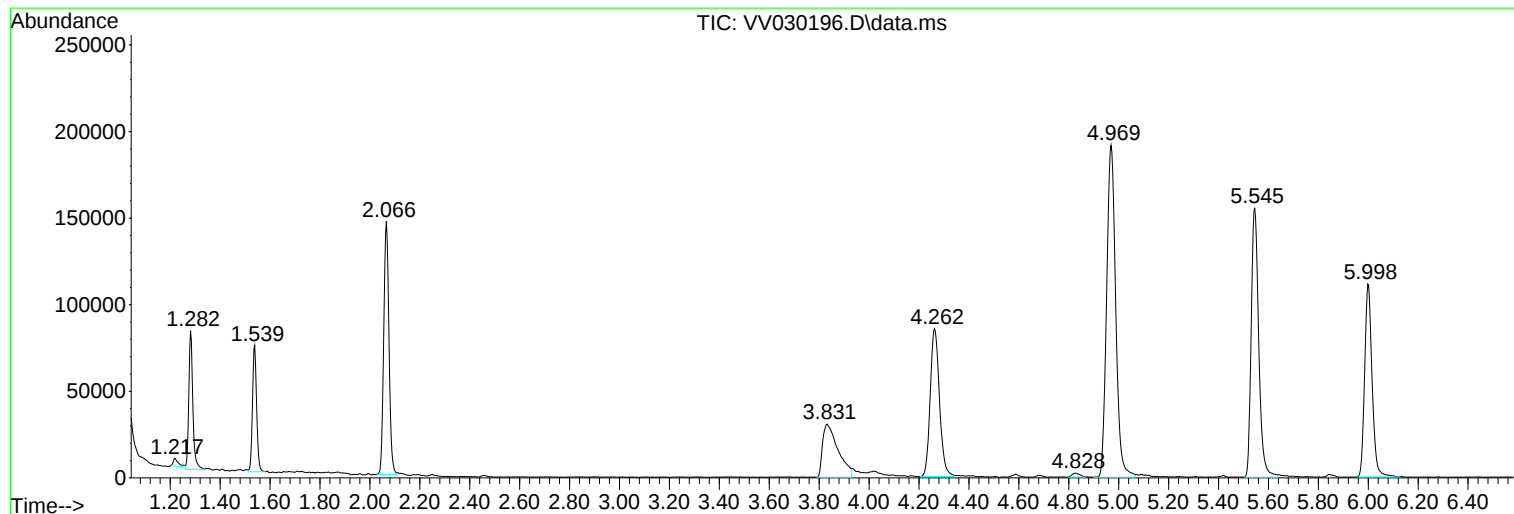

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030196.D
Acq On : 14 Mar 2023 15:35
Operator : SY/MD
Sample : 01906-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030196.D
Acq On : 14 Mar 2023 15:35
Operator : SY/MD
Sample : 01906-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc