

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
 Data File : VV030199.D
 Acq On : 14 Mar 2023 16:45
 Operator : SY/MD
 Sample : 01906-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM97

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	61	rBV	5073	5103	1.18%	0.134%
2	1.281	68	75	92	rVB	71656	82173	19.05%	2.153%
3	1.539	147	155	169	rVB	64244	74779	17.34%	1.960%
4	2.066	309	319	334	rBV	131466	190718	44.22%	4.998%
5	3.825	854	866	900	rBV	34099	124809	28.94%	3.271%
6	4.262	985	1002	1030	rBV2	78179	202043	46.85%	5.295%
7	4.969	1206	1222	1251	rBV3	167632	431274	100.00%	11.302%
8	5.545	1385	1401	1426	rBV	156864	322476	74.77%	8.451%
9	6.002	1529	1543	1570	rBV2	99989	208570	48.36%	5.466%
10	6.924	1818	1830	1849	rBV	42285	80253	18.61%	2.103%
11	7.252	1920	1932	1949	rBV	201188	356386	82.64%	9.339%
12	7.329	1951	1956	1975	rVB	5898	10913	2.53%	0.286%
13	7.564	2019	2029	2048	rBV	26747	47813	11.09%	1.253%
14	7.886	2116	2129	2139	rBV4	5962	11122	2.58%	0.291%
15	8.037	2165	2176	2213	rBV	171687	327357	75.90%	8.579%
16	8.796	2399	2412	2439	rBV	238451	401735	93.15%	10.528%
17	10.162	2826	2837	2854	rBV	79410	123840	28.71%	3.245%
18	10.336	2880	2891	2905	rVB2	21356	34112	7.91%	0.894%
19	11.194	3139	3158	3175	rBV	259481	407225	94.42%	10.672%
20	11.500	3244	3253	3264	rBV3	8506	15930	3.69%	0.417%
21	11.570	3264	3275	3290	rVB	204630	322720	74.83%	8.457%
22	12.204	3459	3472	3487	rBV2	11443	18458	4.28%	0.484%
23	12.297	3492	3501	3509	rBV4	5948	8551	1.98%	0.224%
24	13.998	4020	4030	4040	rVB2	5019	7563	1.75%	0.198%




Sum of corrected areas: 3815923

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030199.D
Acq On : 14 Mar 2023 16:45
Operator : SY/MD
Sample : 01906-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

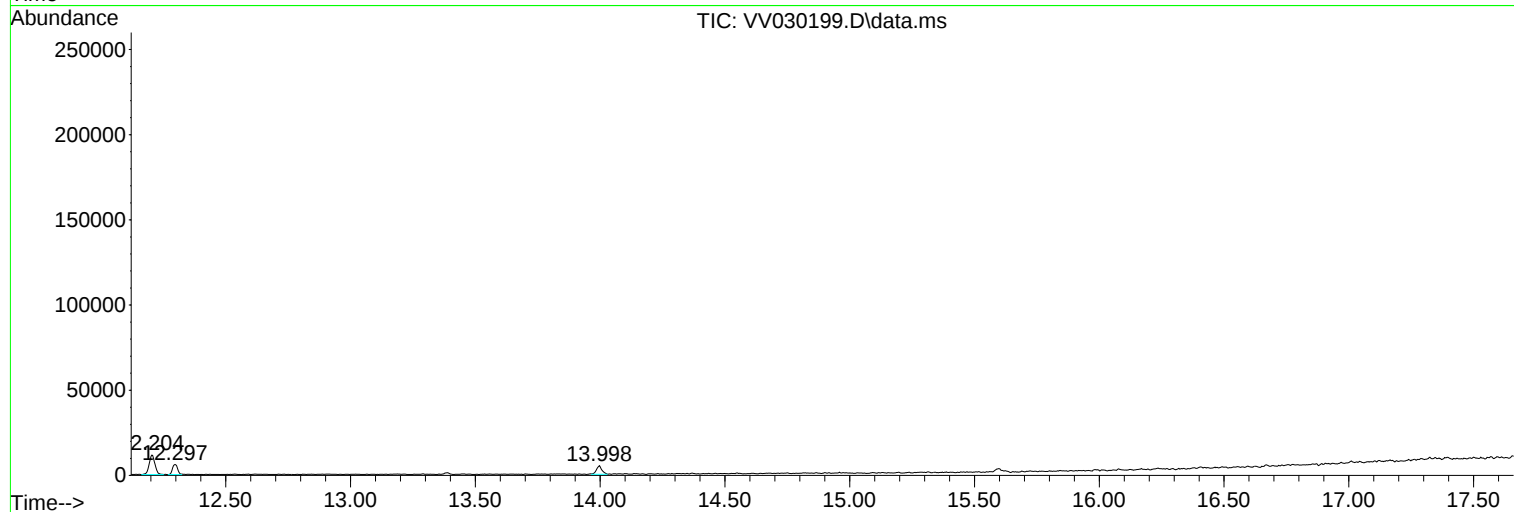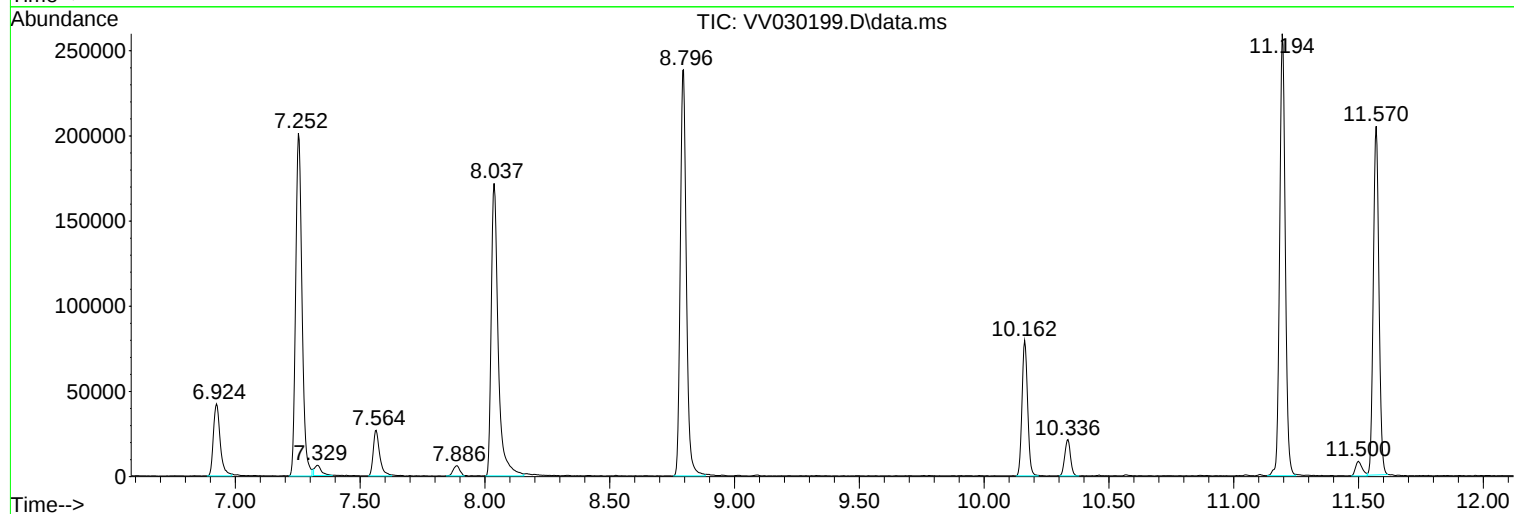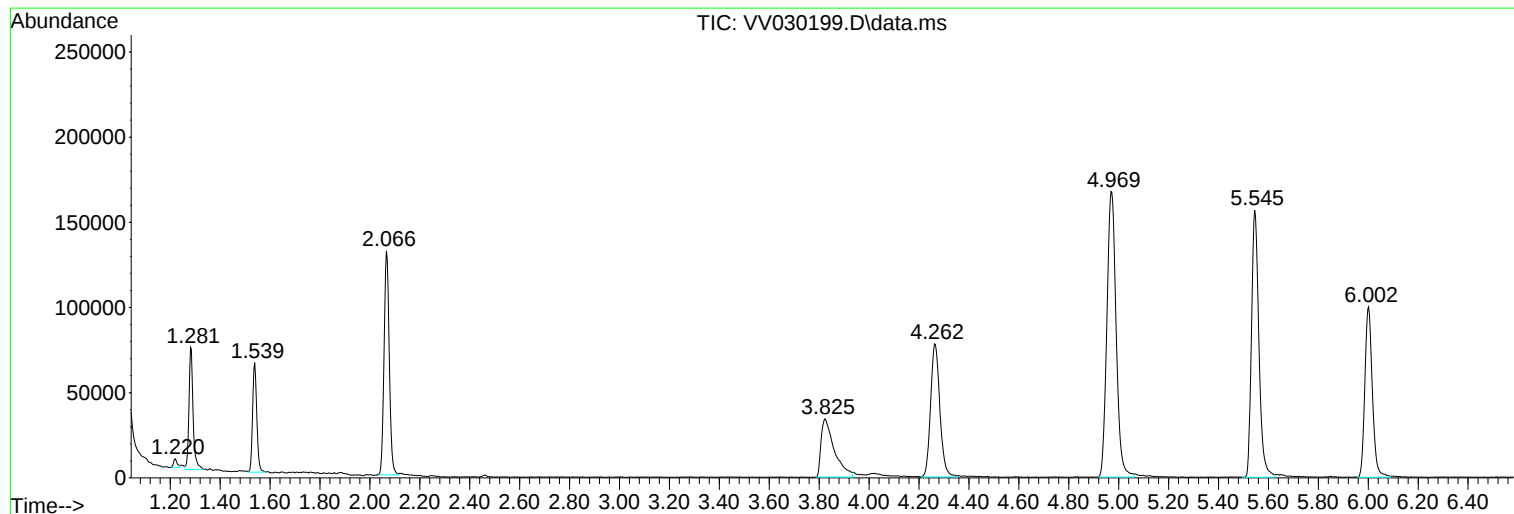

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030199.D
Acq On : 14 Mar 2023 16:45
Operator : SY/MD
Sample : 01906-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030199.D
Acq On : 14 Mar 2023 16:45
Operator : SY/MD
Sample : 01906-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc