

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
 Data File : VV030201.D
 Acq On : 14 Mar 2023 17:33
 Operator : SY/MD
 Sample : VIBLK279
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK279

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	97	rVB	74325	84154	18.88%	2.164%
2	1.539	147	155	168	rVB	66641	78619	17.64%	2.022%
3	2.066	308	319	334	rBV	135355	196450	44.08%	5.052%
4	2.455	426	440	456	rVB	17366	29756	6.68%	0.765%
5	3.825	851	866	911	rBV	36960	144340	32.39%	3.712%
6	4.262	982	1002	1030	rBV	81638	206788	46.40%	5.318%
7	4.969	1205	1222	1249	rBV3	175856	445672	100.00%	11.461%
8	5.545	1388	1401	1425	rBV	152074	313354	70.31%	8.058%
9	5.850	1485	1496	1508	rVB9	4086	8416	1.89%	0.216%
10	5.998	1529	1542	1578	rBV	102565	215594	48.38%	5.544%
11	6.924	1816	1830	1855	rBV	45108	85527	19.19%	2.199%
12	7.252	1920	1932	1966	rBV	208750	374751	84.09%	9.637%
13	7.564	2016	2029	2046	rBV3	26448	48993	10.99%	1.260%
14	7.886	2117	2129	2144	rBV3	7305	13219	2.97%	0.340%
15	8.037	2165	2176	2212	rBV	173933	332153	74.53%	8.541%
16	8.374	2270	2281	2296	rBV2	8102	13996	3.14%	0.360%
17	8.792	2400	2411	2437	rBV	237301	393935	88.39%	10.130%
18	10.162	2826	2837	2857	rBV	80525	126823	28.46%	3.261%
19	10.336	2880	2891	2902	rVB	19363	31235	7.01%	0.803%
20	11.194	3146	3158	3181	rBV	248518	390213	87.56%	10.034%
21	11.570	3263	3275	3292	rBV	211470	330667	74.20%	8.503%
22	12.204	3460	3472	3484	rVB2	15432	24066	5.40%	0.619%




Sum of corrected areas: 3888721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030201.D
Acq On : 14 Mar 2023 17:33
Operator : SY/MD
Sample : VIBLK279
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

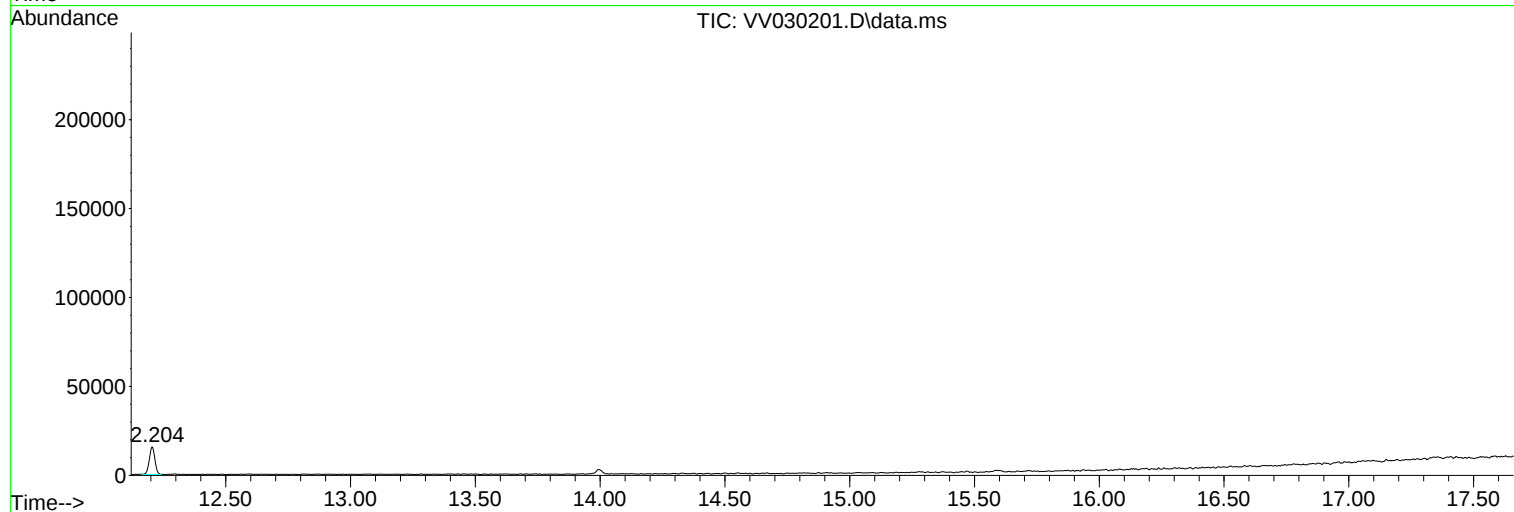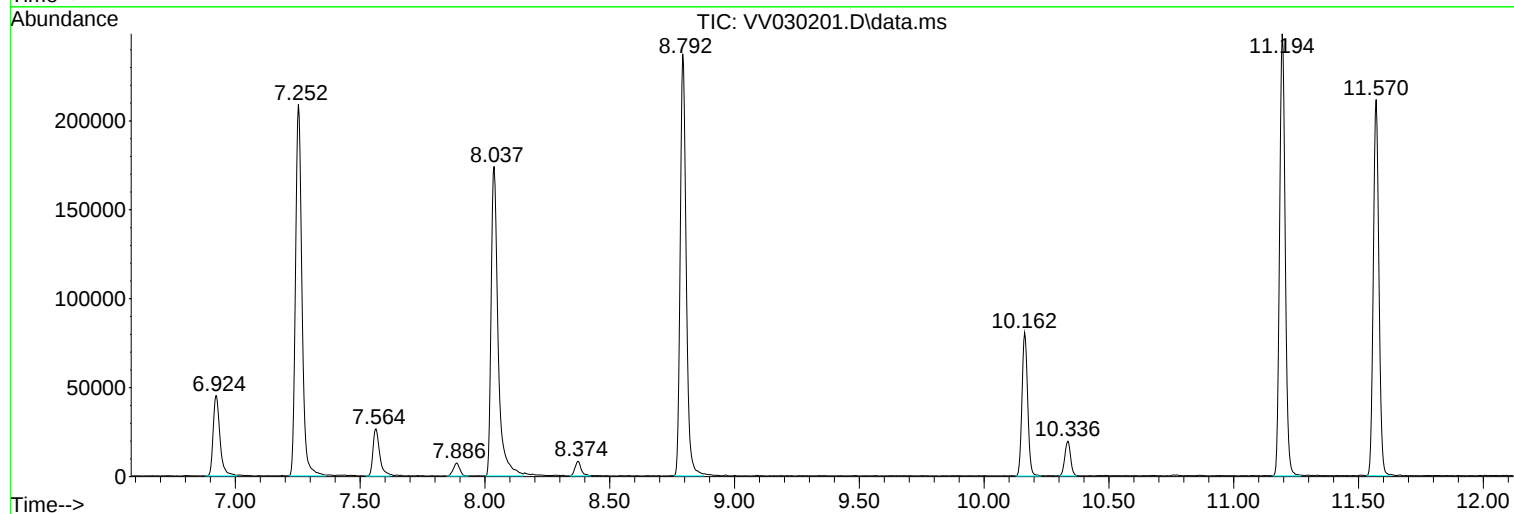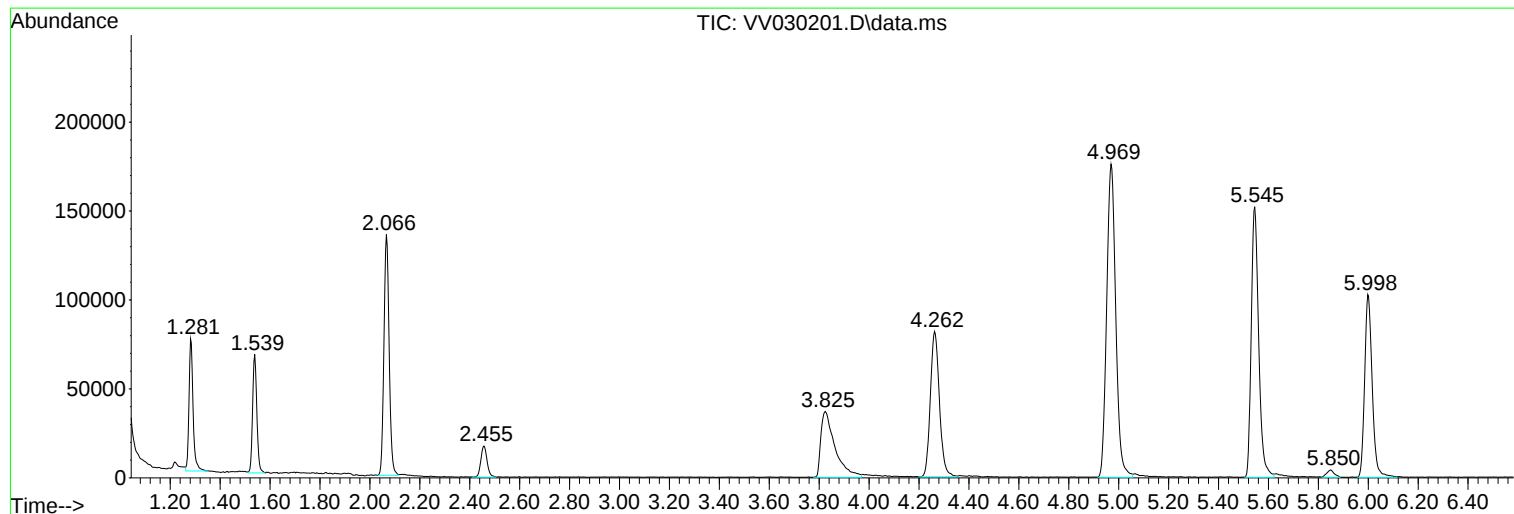

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030201.D
Acq On : 14 Mar 2023 17:33
Operator : SY/MD
Sample : VIBLK279
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030201.D
Acq On : 14 Mar 2023 17:33
Operator : SY/MD
Sample : VIBLK279
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------