


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031423\
Data File : VV030186.D
Acq On : 14 Mar 2023 10:27
Operator : SY/MD
Sample : BFB231
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB231

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Mar 15 01:37:04 2023

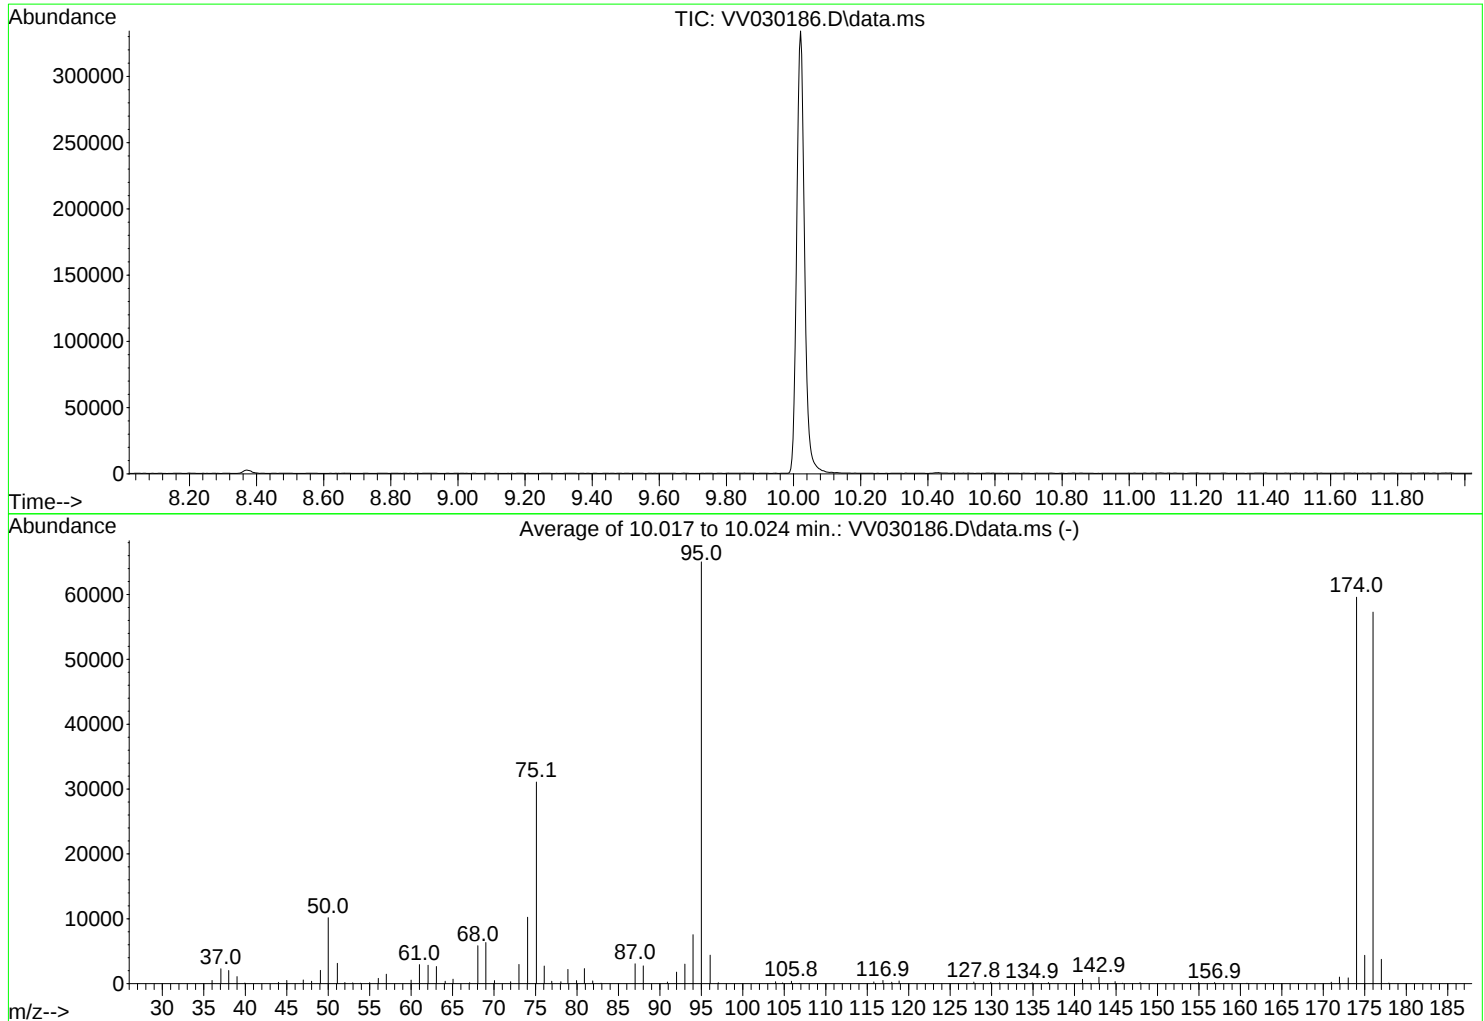

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	10165	PASS
75	95	30	80	47.8	31093	PASS
95	95	100	100	100.0	65032	PASS
96	95	5	9	6.8	4407	PASS
173	174	0.00	2	1.5	880	PASS
174	95	50	120	91.6	59573	PASS
175	174	5	9	7.3	4356	PASS
176	174	95	105	96.2	57293	PASS
177	176	5	10	6.5	3751	PASS

m/z	Abundance
39.90	128.0
44.00	337.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
36.00	486.0
37.00	2389.0
38.00	1998.0
39.00	1117.0
40.00	258.0
44.00	547.0
45.00	504.0
47.00	599.0
48.00	350.0
49.00	2068.0
50.00	10108.0
51.10	3205.0
52.00	146.0
53.00	116.0
53.90	102.0
55.00	116.0
56.10	798.0
57.00	1392.0
60.00	659.0
61.00	2995.0
62.10	2896.0
63.00	2599.0
64.10	385.0
65.00	702.0
67.10	166.0
68.10	5978.0
69.00	6485.0
70.00	481.0
72.00	285.0
73.00	2974.0
74.10	10187.0
75.10	30696.0
76.00	2637.0
77.00	372.0
78.00	274.0
78.90	2166.0
79.90	447.0
80.90	2268.0
81.90	407.0
87.00	3152.0
88.00	2735.0
90.90	231.0
92.00	1865.0
93.00	3110.0
94.00	7510.0
95.00	64152.0
96.10	4471.0
97.10	115.0
104.00	271.0
104.90	101.0
105.90	351.0
115.80	269.0
116.90	500.0
118.00	188.0
118.80	438.0
127.80	258.0
129.90	223.0
131.00	126.0
134.90	148.0
136.90	177.0
140.90	636.0
143.00	977.0
144.90	381.0
145.80	130.0
147.90	163.0
154.90	145.0
156.90	144.0
160.80	102.0
171.00	201.0
172.00	945.0
173.00	859.0
174.00	58304.0
175.00	4374.0
176.00	56024.0
177.00	3591.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
36.00	537.0
37.10	2367.0
38.00	2127.0
39.00	1133.0
40.00	240.0
44.00	539.0
45.00	507.0
47.00	550.0
48.00	398.0
49.00	2099.0
50.00	10457.0
51.10	3197.0
52.00	165.0
53.00	133.0
53.90	101.0
55.00	152.0
56.00	836.0
57.00	1540.0
60.00	553.0
61.00	3051.0
62.00	2953.0
63.10	2716.0
64.10	382.0
65.00	716.0
67.10	152.0
68.00	6036.0
69.00	6527.0
70.10	496.0
72.00	308.0
73.00	3016.0
74.00	10570.0
75.10	32264.0
76.10	2824.0
76.90	393.0
78.00	291.0
78.90	2279.0
80.00	494.0
80.90	2411.0
81.90	443.0
82.90	107.0
87.00	3179.0
88.00	2855.0
90.90	231.0
92.00	1824.0
93.00	3090.0
94.00	7797.0
95.00	67120.0
96.10	4637.0
97.00	153.0
104.00	301.0
104.80	117.0
105.90	387.0
106.80	119.0
115.80	309.0
116.90	512.0
118.00	215.0
118.90	425.0
127.90	243.0
129.90	213.0
130.90	127.0
134.90	135.0
136.90	181.0
140.90	696.0
141.90	116.0
142.90	1033.0
144.90	334.0
145.80	119.0
147.90	195.0
154.90	165.0
156.90	184.0
160.80	109.0
170.90	233.0
172.00	1064.0
173.00	922.0
174.00	61288.0
175.00	4491.0
176.00	59080.0
177.00	3865.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
36.00	472.0
37.00	2152.0
38.00	1975.0
39.00	1009.0
40.00	208.0
44.00	522.0
45.00	508.0
47.00	581.0
48.00	367.0
49.10	1975.0
50.00	9930.0
51.10	2969.0
52.00	182.0
52.90	113.0
55.00	170.0
56.00	792.0
57.00	1465.0
60.00	435.0
61.00	2778.0
62.00	2654.0
63.10	2622.0
64.10	345.0
65.10	642.0
67.00	107.0
68.00	5509.0
69.00	5993.0
70.00	454.0
72.00	329.0
73.00	2875.0
74.00	9982.0
75.10	30320.0
76.10	2661.0
76.90	369.0
78.10	301.0
78.90	2168.0
80.00	509.0
80.90	2261.0
81.90	408.0
82.90	118.0
87.00	2892.0
88.00	2625.0
90.90	247.0
92.00	1664.0
93.00	2823.0
94.00	7345.0
95.00	63824.0
96.00	4113.0
97.00	161.0
103.90	325.0
104.70	135.0
105.80	388.0
115.80	282.0
116.90	468.0
117.90	235.0
118.90	418.0
127.90	234.0
129.90	196.0
130.90	107.0
134.90	108.0
136.80	172.0
141.00	649.0
141.90	114.0
142.90	977.0
144.90	274.0
147.90	187.0
155.00	148.0
156.90	185.0
170.90	231.0
171.90	1064.0
173.00	858.0
174.00	59128.0
175.00	4204.0
176.00	56776.0
177.00	3797.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231