


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031519\
Data File : VV009678.D
Acq On : 15 Mar 2019 09:37
Operator : SY/MD
Sample : BFB77
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM031319S.M
Title : VOC Analysis
Last Update : Fri Mar 15 22:56:00 2019

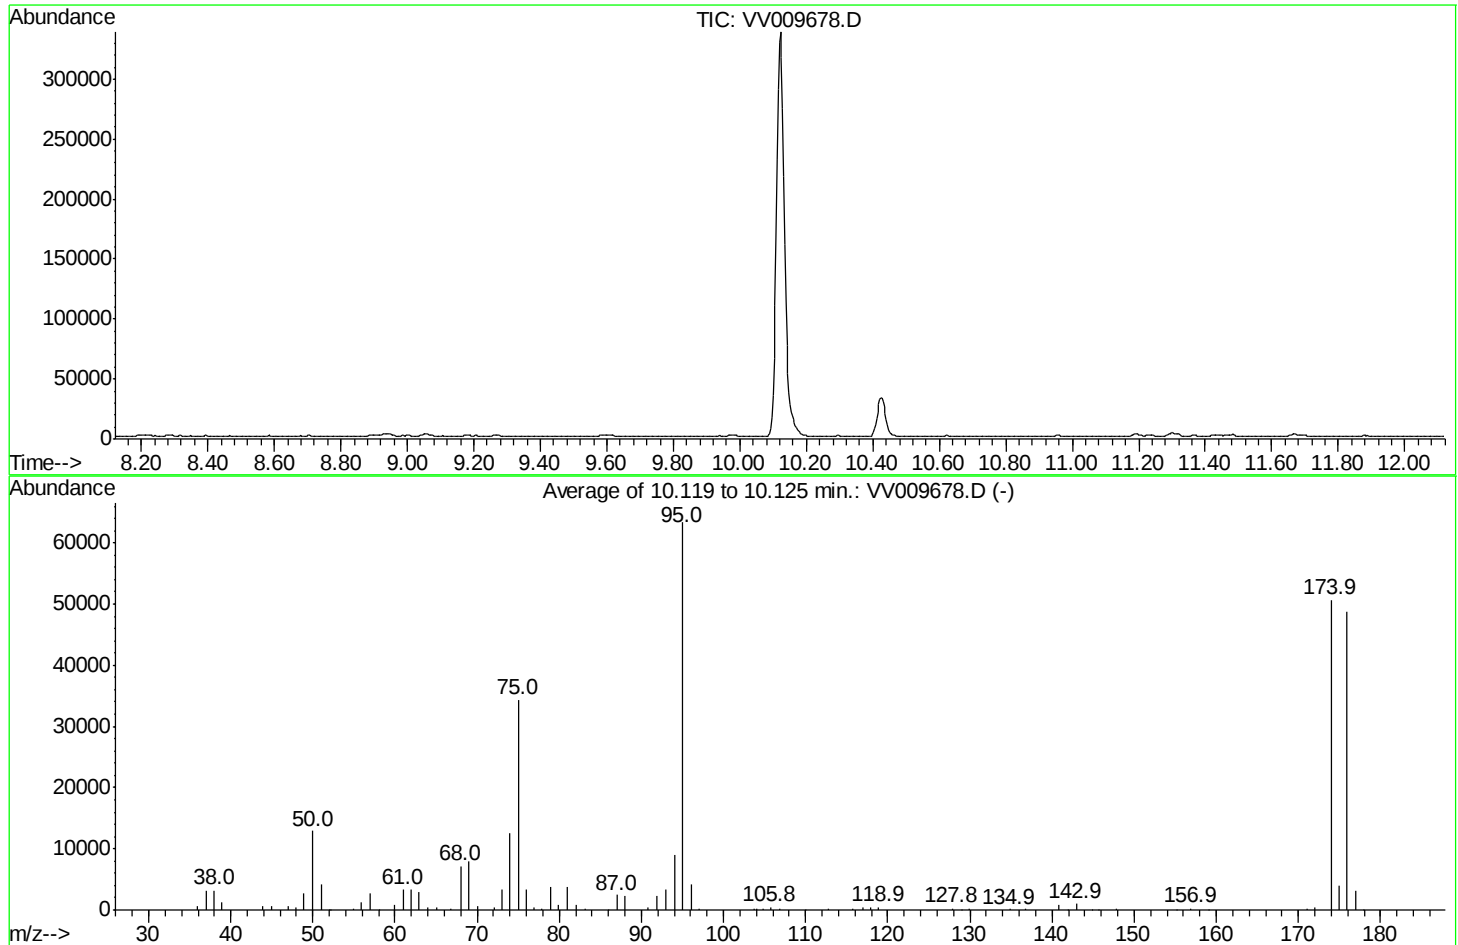

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	12908	PASS
75	95	30	80	54.3	34386	PASS
95	95	100	100	100.0	63352	PASS
96	95	5	9	6.5	4131	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.1	50714	PASS
175	174	5	9	8.0	4064	PASS
176	174	95	101	96.1	48752	PASS
177	176	5	9	6.4	3137	PASS

Scan 2796 (10.080 min): VV009678.D
BFB77

m/z	Abundance
39.90	2182.0
43.70	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	559.0
37.00	3204.0
38.00	3245.0
38.90	1439.0
39.90	2058.0
43.90	814.0
44.90	635.0
47.00	695.0
47.90	436.0
48.90	2969.0
50.00	13261.0
51.00	4081.0
51.90	148.0
54.90	242.0
55.90	1334.0
57.00	2817.0
59.90	738.0
61.00	3323.0
62.00	3362.0
63.00	2941.0
63.90	402.0
65.10	384.0
66.90	159.0
68.00	7572.0
69.00	8002.0
70.00	628.0
72.10	370.0
73.00	3079.0
74.00	12909.0
75.00	35120.0
76.00	3444.0
76.90	531.0
77.90	252.0
78.90	3765.0
79.80	912.0
80.90	3823.0
82.00	898.0
83.10	147.0
85.90	106.0
87.00	2485.0
87.90	2435.0
90.80	462.0
91.90	2173.0
93.00	3214.0
94.00	8992.0
95.00	63368.0
96.10	4134.0
97.00	138.0
104.10	395.0
104.90	193.0
105.80	463.0
106.80	141.0
112.80	131.0
115.80	284.0
117.00	474.0
117.90	385.0
118.90	472.0
127.90	246.0
129.90	237.0
134.90	250.0
136.70	134.0
140.90	912.0
143.00	1042.0
144.90	129.0
147.90	188.0
155.10	153.0
156.90	230.0
159.00	132.0
171.10	110.0
172.00	476.0
174.00	50280.0
175.00	4032.0
175.90	47736.0
176.90	3143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	576.0
37.00	3199.0
38.00	3216.0
38.90	1394.0
39.90	1988.0
43.90	891.0
45.00	663.0
47.00	620.0
47.90	417.0
48.90	2859.0
50.00	13373.0
51.00	4231.0
52.20	123.0
54.90	252.0
55.90	1228.0
57.00	2861.0
58.10	148.0
59.90	786.0
61.00	3391.0
61.90	3456.0
63.00	2966.0
63.90	417.0
65.00	332.0
66.90	147.0
68.00	7308.0
69.00	8207.0
70.00	639.0
72.00	394.0
73.00	3394.0
74.00	12840.0
75.00	35232.0
76.00	3464.0
76.90	522.0
77.90	234.0
78.90	3940.0
79.80	837.0
80.90	3875.0
82.00	971.0
83.10	192.0
85.90	107.0
87.00	2531.0
87.90	2513.0
90.80	420.0
91.90	2251.0
93.00	3352.0
94.00	9192.0
95.00	65448.0
96.10	4266.0
97.00	162.0
103.70	386.0
104.80	205.0
105.80	487.0
106.80	137.0
110.00	103.0
112.70	125.0
115.80	289.0
116.90	496.0
117.90	440.0
118.90	501.0
127.80	242.0
129.00	115.0
129.90	250.0
134.90	212.0
136.70	141.0
140.90	951.0
143.00	1010.0
144.90	120.0
145.70	107.0
147.90	218.0
155.10	120.0
156.90	230.0
159.00	131.0
171.10	115.0
172.00	545.0
174.00	52176.0
175.00	4188.0
176.00	50144.0
177.00	3229.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	525.0
37.00	2900.0
38.00	2981.0
38.90	1133.0
39.90	1986.0
43.90	859.0
45.00	638.0
46.90	471.0
47.80	393.0
48.90	2414.0
50.00	12091.0
51.00	3979.0
54.90	246.0
56.00	1189.0
57.00	2551.0
58.10	169.0
59.90	770.0
61.00	3291.0
61.90	3263.0
62.90	2848.0
64.00	383.0
65.00	257.0
66.80	135.0
68.00	6472.0
69.00	7470.0
70.10	594.0
72.00	348.0
73.00	3355.0
74.00	11689.0
75.00	32808.0
76.00	3097.0
76.90	482.0
77.80	264.0
78.90	3750.0
79.90	791.0
80.90	3753.0
82.00	870.0
83.10	182.0
87.00	2360.0
88.00	2281.0
90.80	389.0
91.90	2233.0
93.00	3243.0
94.00	8565.0
95.00	61240.0
96.00	3993.0
97.00	140.0
103.70	425.0
104.80	189.0
105.70	469.0
106.80	117.0
110.00	112.0
112.70	116.0
115.80	256.0
116.80	520.0
117.90	446.0
118.90	518.0
127.80	241.0
128.90	151.0
129.90	232.0
134.90	156.0
136.80	141.0
140.90	931.0
141.90	135.0
142.90	965.0
145.70	110.0
147.90	194.0
156.90	195.0
171.00	116.0
172.00	567.0
173.90	49688.0
175.00	3973.0
176.00	48376.0
177.00	3040.0
177.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77