

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V031521\
Data File : VV020607.D
Acq On : 15 Mar 2021 16:19
Operator : SY/MD
Sample : M1633-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B69

Manual Integrations
APPROVED

MMDadoda
3/16/2021 4:35:39 PM

Quant Time: Mar 16 03:46:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 16 03:42:12 2021
Response via : Initial Calibration

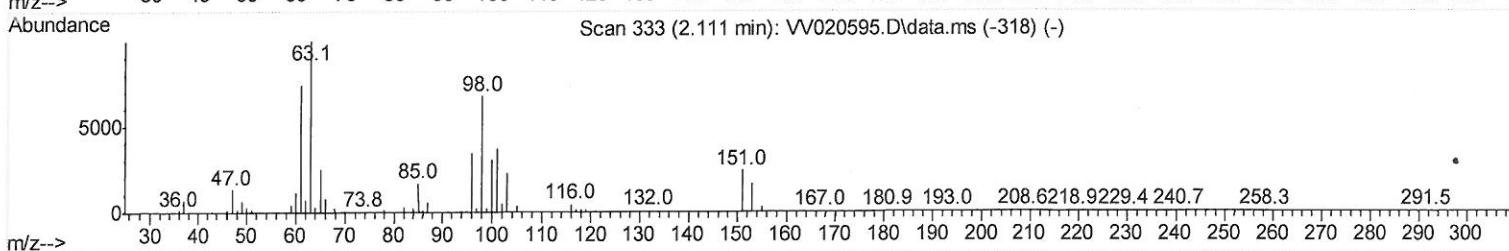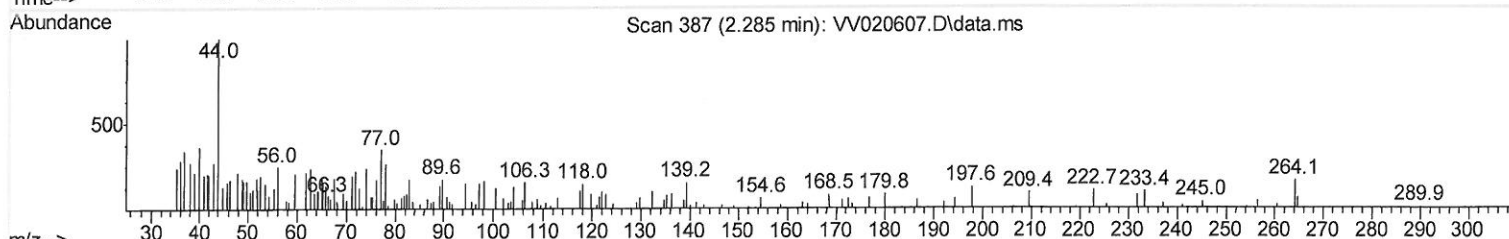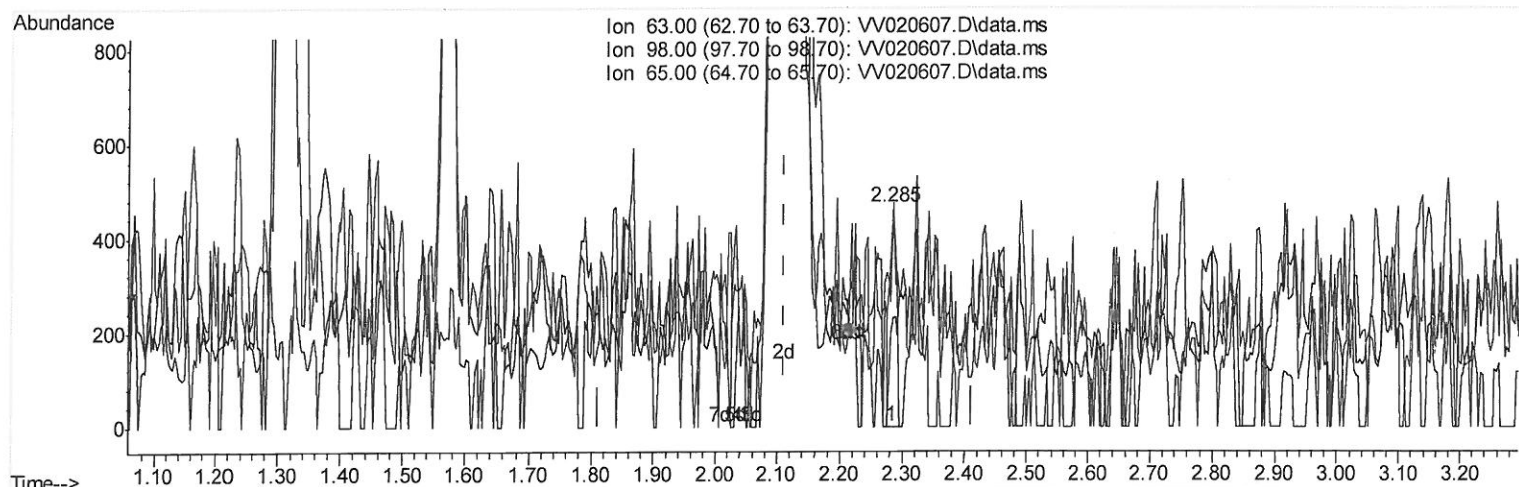

TIC: VV020607.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.285min (+ 0.174) 0.05 ug/L

response 348

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.80	54.60
65.00	23.90	29.31
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V031521\
Data File : VV020607.D
Acq On : 15 Mar 2021 16:19
Operator : SY/MD
Sample : M1633-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B69

Manual Integrations
APPROVED

MMDadoda
3/16/2021 4:35:39 PM

Quant Time: Mar 16 03:46:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 16 03:42:12 2021
Response via : Initial Calibration

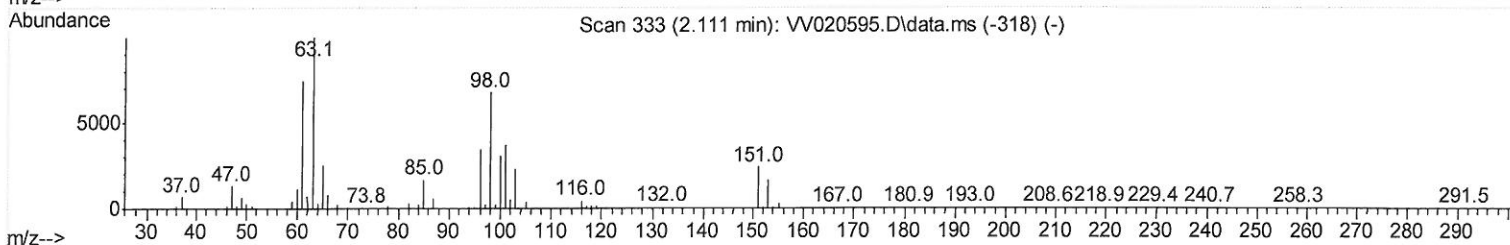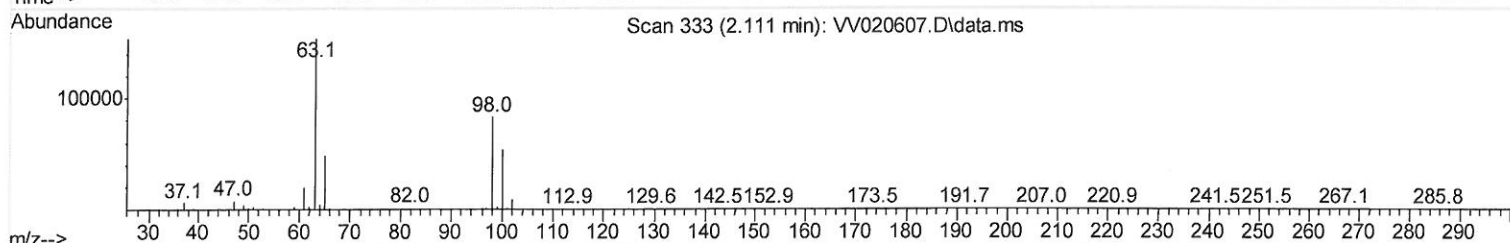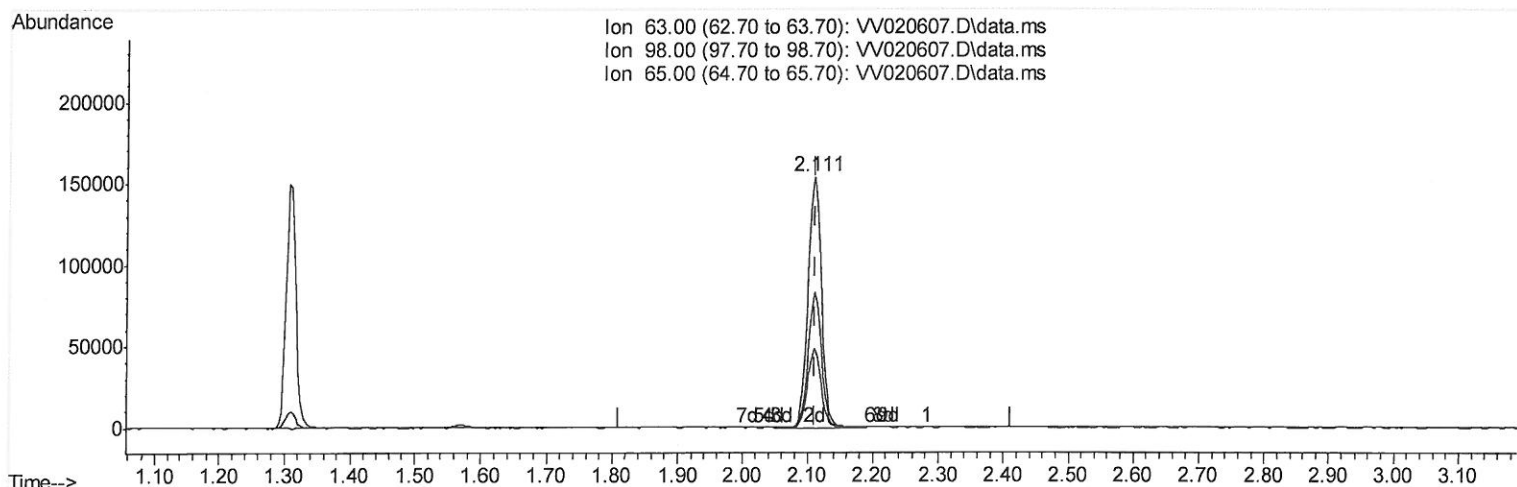

TIC: VV020607.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.111min (-0.000) 30.54 ug/L m

response 221853

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.80	0.09#
65.00	23.90	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V031521\
 Data File : V020607.D
 Acq On : 15 Mar 2021 16:19
 Operator : SY/MD
 Sample : M1633-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B69

Manual Integrations
 APPROVED

MMDadoda
 3/16/2021 4:35:39 PM

Quant Time: Mar 16 03:46:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 16 03:42:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	473802	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	460687	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	201406	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	151062	39.53	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.06%		
7) Chloroethane-d5	1.571	69	130878	42.80	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	85.60%		
11) 1,1-Dichloroethene-d2	2.111	63	221853m	30.54	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.08%		
21) 2-Butanone-d5	3.889	46	267117	108.90	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.90%		
24) Chloroform-d	4.352	84	295075	44.42	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.84%		
26) 1,2-Dichloroethane-d4	5.034	65	211924	48.35	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.70%		
32) Benzene-d6	5.053	84	595036	46.75	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.50%		
36) 1,2-Dichloropropane-d6	6.072	67	195375	47.98	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.96%		
41) Toluene-d8	7.320	98	503272	44.49	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.98%		
43) trans-1,3-Dichloroprop...	7.625	79	83253	43.74	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.48%		
47) 2-Hexanone-d5	8.092	63	151296	99.30	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	99.30%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	241315	47.42	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.84%		
64) 1,2-Dichlorobenzene-d4	11.632	152	196585	50.37	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.74%		
Target Compounds						Qvalue
25) Chloroform	4.381	83	14086	2.07	ug/L	93
34) Trichloroethene	5.921	95	5597	1.43	ug/L	86
48) 2-Hexanone	8.149	43	9808	2.30	ug/L #	50

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031521\
Data File : VW020607.D
Acq On : 15 Mar 2021 16:19
Operator : SY/MD
Sample : M1633-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B69

Manual Integrations
APPROVED

MMDadoda
3/16/2021 4:35:39 PM

Quant Time: Mar 16 03:46:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 16 03:42:12 2021
Response via : Initial Calibration

