

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031521\
 Data File : VV020601.D
 Acq On : 15 Mar 2021 13:30
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

Signal : TIC: VV020601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	97	rVB	249150	257006	13.93%	1.893%
2	1.571	158	165	177	rVB	228457	256270	13.89%	1.888%
3	2.111	324	333	354	rVB	408580	619752	33.59%	4.566%
4	2.285	384	387	388	rBV3	4069	2403	0.13%	0.018%
5	2.323	397	399	403	rBV5	3843	2659	0.14%	0.020%
6	2.439	432	435	438	rBV5	4344	2664	0.14%	0.020%
7	2.590	479	482	484	rBV4	4407	2788	0.15%	0.021%
8	2.760	530	535	536	rBV5	4972	3852	0.21%	0.028%
9	2.799	540	547	551	rBV8	5576	6412	0.35%	0.047%
10	2.847	558	562	563	rBV4	4862	2936	0.16%	0.022%
11	2.867	565	568	571	rVB5	4223	2665	0.14%	0.020%
12	2.937	587	590	592	rBV4	3649	2243	0.12%	0.017%
13	3.127	646	649	651	rBV4	4437	1986	0.11%	0.015%
14	3.236	679	683	689	rBV8	4526	4032	0.22%	0.030%
15	3.346	714	717	721	rBV6	4856	3697	0.20%	0.027%
16	3.365	721	723	727	rBV5	2701	2124	0.12%	0.016%
17	3.400	731	734	737	rBV5	3361	2348	0.13%	0.017%
18	3.613	798	800	804	rVB4	3861	2402	0.13%	0.018%
19	3.838	866	870	871	rBV4	2916	1929	0.10%	0.014%
20	3.889	877	886	915	rBV	126332	365219	19.80%	2.691%
21	4.082	944	946	949	rBV4	5116	2352	0.13%	0.017%
22	4.352	1015	1030	1054	rBV	310583	748097	40.55%	5.512%
23	4.468	1062	1066	1069	rBV6	6314	5307	0.29%	0.039%
24	4.654	1119	1124	1129	rBV9	3626	4297	0.23%	0.032%
25	4.857	1185	1187	1190	rVB4	4797	2165	0.12%	0.016%
26	4.883	1190	1195	1198	rBV6	4217	3959	0.21%	0.029%
27	4.899	1198	1200	1204	rBV4	3799	2430	0.13%	0.018%
28	5.050	1231	1247	1268	rBV3	716636	1844934	100.00%	13.593%
29	5.294	1319	1323	1324	rBV3	3462	2025	0.11%	0.015%
30	5.410	1353	1359	1364	rBV10	5236	7804	0.42%	0.057%
31	5.619	1413	1424	1445	rBV	515629	1021965	55.39%	7.529%
32	6.075	1555	1566	1592	rVB	414851	846236	45.87%	6.235%
33	6.587	1723	1725	1729	rVB4	6294	3620	0.20%	0.027%
34	6.657	1745	1747	1749	rBV3	3706	1923	0.10%	0.014%
35	6.731	1767	1770	1771	rBV3	3788	2044	0.11%	0.015%
36	6.989	1841	1850	1869	rVV	226854	405261	21.97%	2.986%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031521\
 Data File : VV020601.D
 Acq On : 15 Mar 2021 13:30
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Title : VOC Analysis

37	7.220	1919	1922	1925	rBV4	3584	3087	0.17%	0.023%
38	7.320	1942	1953	1971	rBV	789334	1350780	73.22%	9.952%
39	7.625	2039	2048	2070	rVB	161220	283753	15.38%	2.091%
40	7.937	2142	2145	2147	rBV4	4779	3124	0.17%	0.023%
41	8.091	2184	2193	2220	rBV2	419096	819537	44.42%	6.038%
42	8.506	2319	2322	2323	rBV3	3173	2001	0.11%	0.015%
43	8.542	2330	2333	2338	rBV7	4901	5217	0.28%	0.038%
44	8.587	2345	2347	2353	rVB7	4590	3980	0.22%	0.029%
45	8.622	2353	2358	2361	rBV7	4586	3326	0.18%	0.025%
46	8.763	2398	2402	2404	rBV4	3754	3198	0.17%	0.024%
47	8.857	2420	2431	2448	rBV	813880	1302399	70.59%	9.595%
48	9.226	2544	2546	2549	rVB3	5730	2662	0.14%	0.020%
49	9.255	2549	2555	2556	rBV6	4704	4147	0.22%	0.031%
50	9.371	2586	2591	2593	rBV6	4010	2982	0.16%	0.022%
51	9.519	2635	2637	2641	rBV4	2492	2194	0.12%	0.016%
52	9.651	2675	2678	2681	rBV5	4925	4548	0.25%	0.034%
53	9.754	2707	2710	2711	rBV3	3220	2070	0.11%	0.015%
54	9.818	2728	2730	2734	rBV4	3549	2353	0.13%	0.017%
55	9.860	2741	2743	2745	rBV3	3926	1895	0.10%	0.014%
56	9.882	2745	2750	2756	rVV9	4237	6302	0.34%	0.046%
57	10.223	2842	2856	2873	rBV	499500	799853	43.35%	5.893%
58	10.297	2876	2879	2881	rBV4	5215	3663	0.20%	0.027%
59	10.442	2921	2924	2927	rVB5	3523	2270	0.12%	0.017%
60	10.484	2935	2937	2940	rBV4	4374	2678	0.15%	0.020%
61	10.551	2955	2958	2966	rVB10	3783	3801	0.21%	0.028%
62	10.699	3000	3004	3005	rBV4	3938	2859	0.15%	0.021%
63	11.255	3167	3177	3193	rVB	763221	1179727	63.94%	8.692%
64	11.477	3243	3246	3248	rBV4	3965	2585	0.14%	0.019%
65	11.632	3283	3294	3310	rBV	784596	1203875	65.25%	8.870%
66	11.934	3385	3388	3391	rBV5	4249	2745	0.15%	0.020%
67	12.075	3430	3432	3437	rBV6	2763	2270	0.12%	0.017%
68	12.114	3441	3444	3447	rVV5	3306	2376	0.13%	0.018%
69	12.133	3447	3450	3455	rVB6	4705	3799	0.21%	0.028%
70	12.294	3495	3500	3502	rBV5	3686	3748	0.20%	0.028%
71	12.339	3508	3514	3516	rBV7	4242	4150	0.22%	0.031%
72	12.361	3518	3521	3525	rBV5	4036	2966	0.16%	0.022%
73	12.432	3541	3543	3545	rBV3	3803	1867	0.10%	0.014%
74	12.464	3552	3553	3558	rVB5	3184	1890	0.10%	0.014%
75	12.545	3576	3578	3582	rBV5	4238	2956	0.16%	0.022%
76	12.590	3589	3592	3596	rBV5	3883	3701	0.20%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031521\
 Data File : VV020601.D
 Acq On : 15 Mar 2021 13:30
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Title : VOC Analysis

77	12.837	3667	3669	3674	rVB5	3885	2568	0.14%	0.019%
78	12.866	3674	3678	3681	rBV7	4026	3538	0.19%	0.026%
79	12.918	3690	3694	3696	rBV4	4685	3781	0.20%	0.028%
80	13.008	3720	3722	3727	rVB6	3674	2591	0.14%	0.019%
81	13.075	3740	3743	3747	rBV6	2766	2084	0.11%	0.015%
82	13.104	3747	3752	3754	rBV5	2444	2522	0.14%	0.019%
83	13.275	3795	3805	3811	rBV5	11483	19897	1.08%	0.147%
84	13.323	3817	3820	3824	rVB5	4070	3247	0.18%	0.024%
85	13.374	3833	3836	3839	rVB5	3447	1988	0.11%	0.015%
86	13.943	4011	4013	4019	rVB6	2725	2470	0.13%	0.018%
87	14.133	4069	4072	4076	rBV6	4699	3775	0.20%	0.028%
88	14.426	4162	4163	4165	rBV2	3774	1922	0.10%	0.014%
89	14.516	4188	4191	4194	rBV5	2764	1905	0.10%	0.014%
90	14.612	4219	4221	4225	rVB5	3902	2174	0.12%	0.016%
91	14.651	4230	4233	4237	rVV5	4319	2652	0.14%	0.020%
92	14.805	4279	4281	4286	rVB6	3828	2865	0.16%	0.021%
93	14.831	4286	4289	4290	rBV2	3851	2132	0.12%	0.016%
94	14.943	4322	4324	4329	rVB6	3956	2091	0.11%	0.015%
95	15.120	4377	4379	4383	rBV4	4085	3533	0.19%	0.026%
96	15.258	4420	4422	4424	rVB3	6122	2479	0.13%	0.018%
97	15.274	4424	4427	4428	rBV3	4709	2467	0.13%	0.018%
98	15.390	4461	4463	4466	rVB4	4386	2441	0.13%	0.018%
99	15.464	4483	4486	4490	rBV5	4105	2268	0.12%	0.017%
100	15.905	4621	4623	4625	rBV3	4978	2545	0.14%	0.019%


Sum of corrected areas: 13573075

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031521\
Data File : VV020601.D
Acq On : 15 Mar 2021 13:30
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

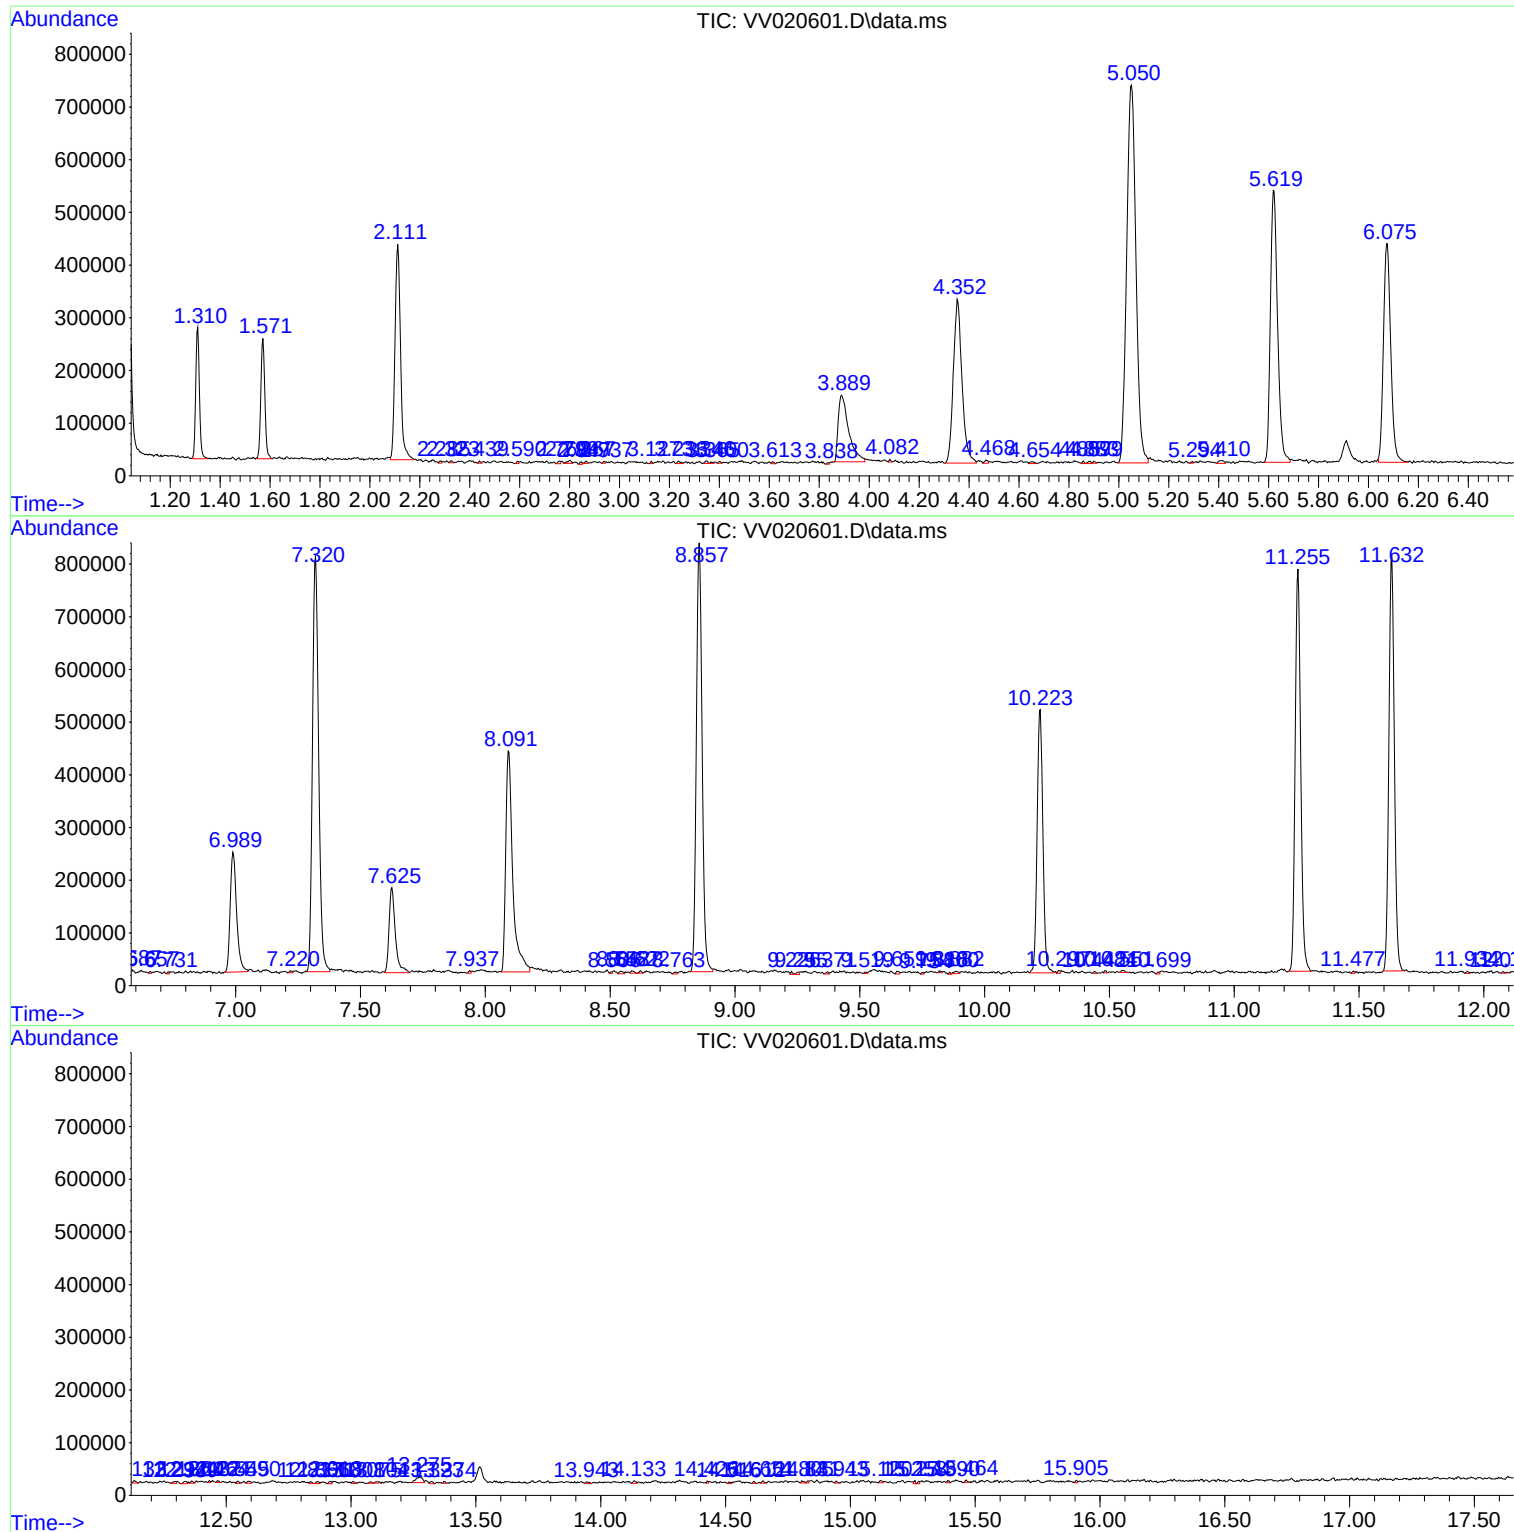

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031521\
Data File : VV020601.D
Acq On : 15 Mar 2021 13:30
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031521\
Data File : VV020601.D
Acq On : 15 Mar 2021 13:30
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
