




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030207.D
 Acq On : 15 Mar 2023 13:24
 Operator : SY/MD
 Sample : 01884-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB918

Manual IntegrationsAPPROVED

Quant Time: Mar 16 01:51:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 16 01:47:11 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

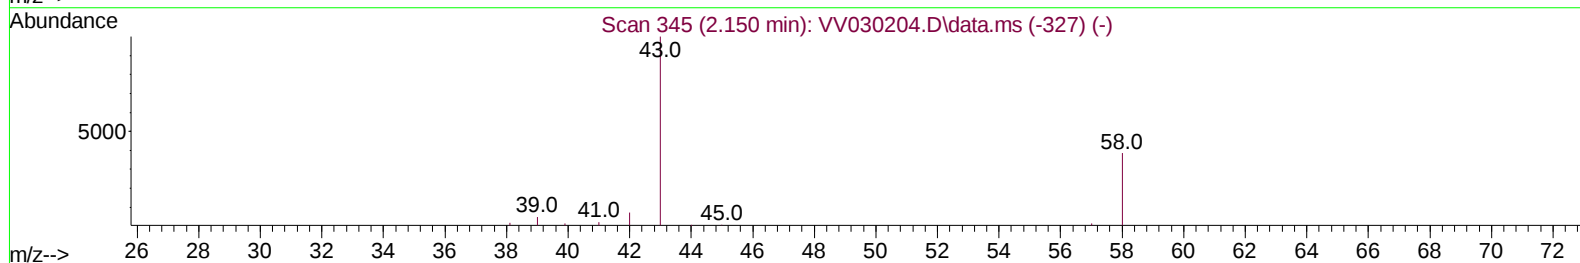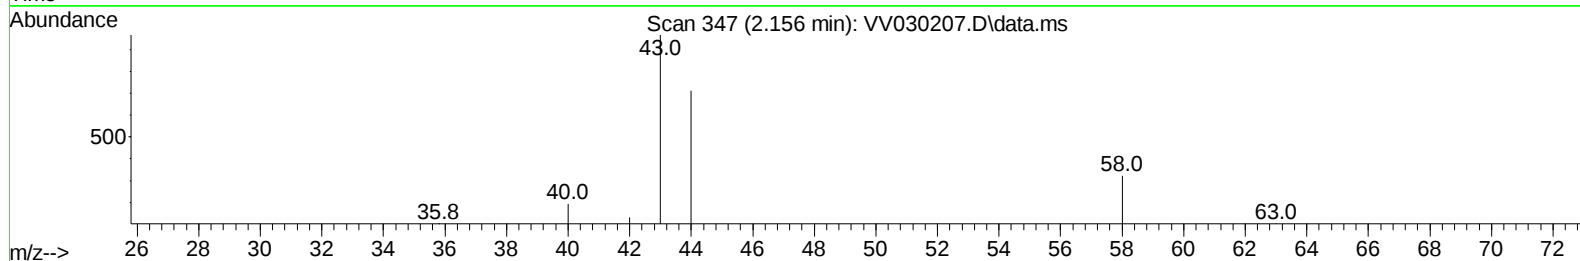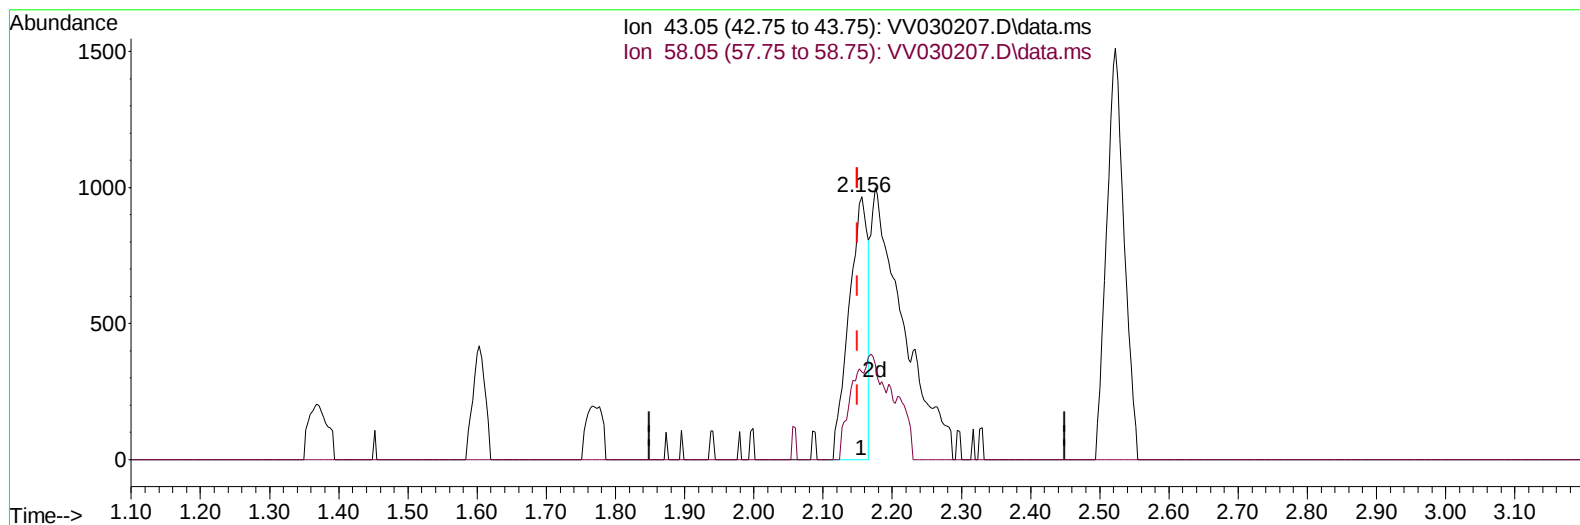

TIC: VV030207.D\data.ms

(13) Acetone (T)

2.156min (+ 0.006) 1.47 ug/L

response 1830

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	28.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030207.D
 Acq On : 15 Mar 2023 13:24
 Operator : SY/MD
 Sample : 01884-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB918

Manual IntegrationsAPPROVED

Quant Time: Mar 16 01:51:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 16 01:47:11 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

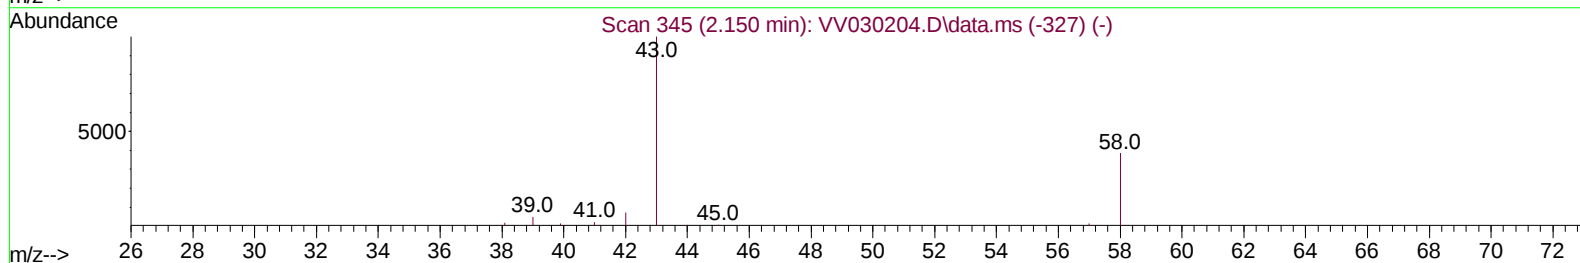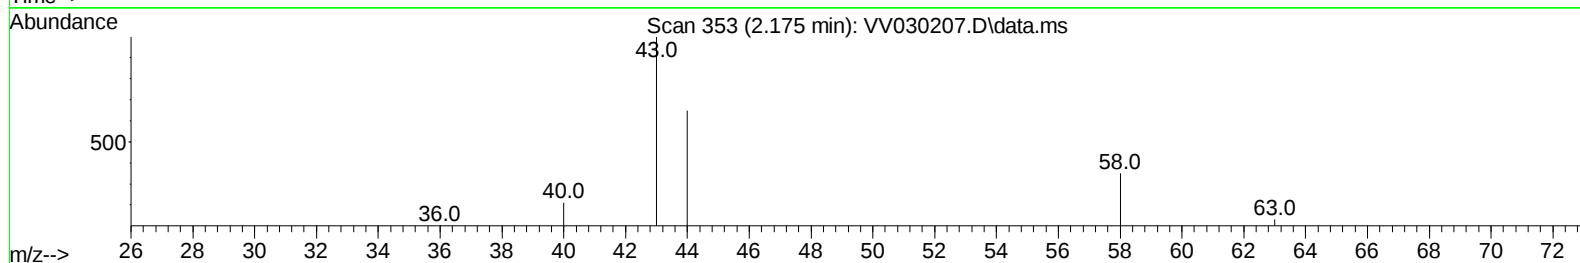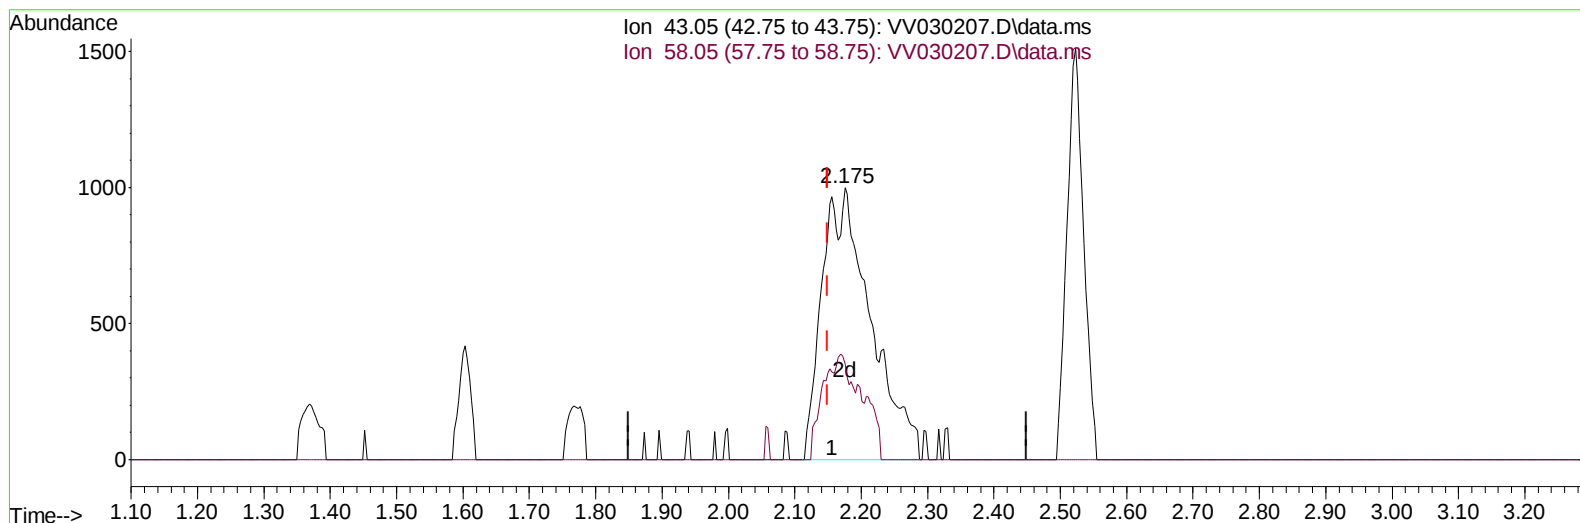

TIC: VV030207.D\data.ms

(13) Acetone (T)

2.175min (+ 0.026) 4.10 ug/L m

response 5089

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	10.32
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030207.D
 Acq On : 15 Mar 2023 13:24
 Operator : SY/MD
 Sample : 01884-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB918

Manual IntegrationsAPPROVED

Quant Time: Mar 16 01:51:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 16 01:47:11 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		140810	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		142754	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		70582	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		44362	4.869	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.400%	
7) Chloroethane-d5	1.539	69		41352	4.835	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.800%	
11) 1,1-Dichloroethene-d2	2.066	63		68971	3.682	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.600%	
20) 2-Butanone-d5	3.834	46		69502	41.375	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.740%	
24) Chloroform-d	4.259	84		87788	4.717	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%	
26) 1,2-Dichloroethane-d4	4.953	65		37404	4.923	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%	
32) Benzene-d6	4.973	84		158994	4.139	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%	
36) 1,2-Dichloropropane-d6	5.998	67		49890	4.317	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.400%	
41) Toluene-d8	7.252	98		135638	3.725	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.600%	
43) trans-1,3-Dichloroprop...	7.561	79		16672	4.217	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.400%	
46) 2-Hexanone-d5	8.037	63		62252	38.059	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.120%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		36439	4.432	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%	
66) 1,2-Dichlorobenzene-d4	11.570	152		55278	4.629	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.600%	
Target Compounds							
13) Acetone	2.175	43		5089m	4.099	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030207.D
Acq On : 15 Mar 2023 13:24
Operator : SY/MD
Sample : 01884-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB918

Manual IntegrationsAPPROVED

Quant Time: Mar 16 01:51:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 16 01:47:11 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
Supervised By :Mahesh Dadoda 03/17/2023

