




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030212.D
 Acq On : 15 Mar 2023 15:24
 Operator : SY/MD
 Sample : 01884-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB919

Manual IntegrationsAPPROVED

Quant Time: Mar 16 01:52:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 16 01:47:11 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

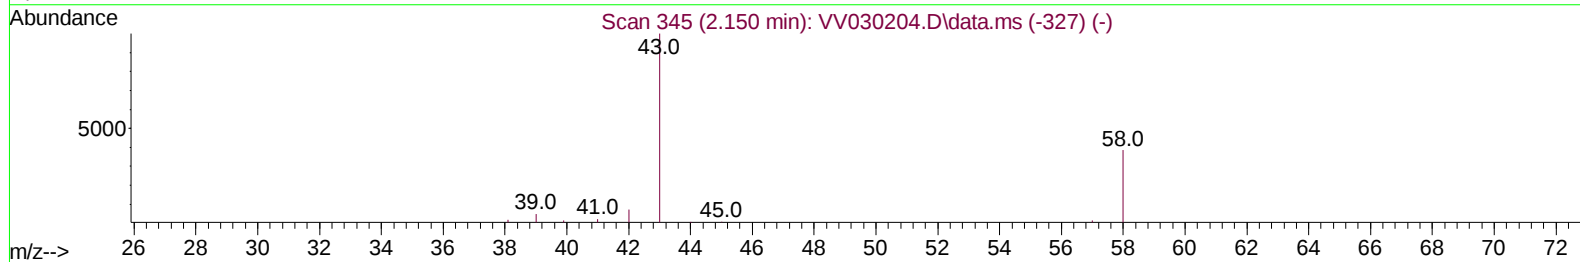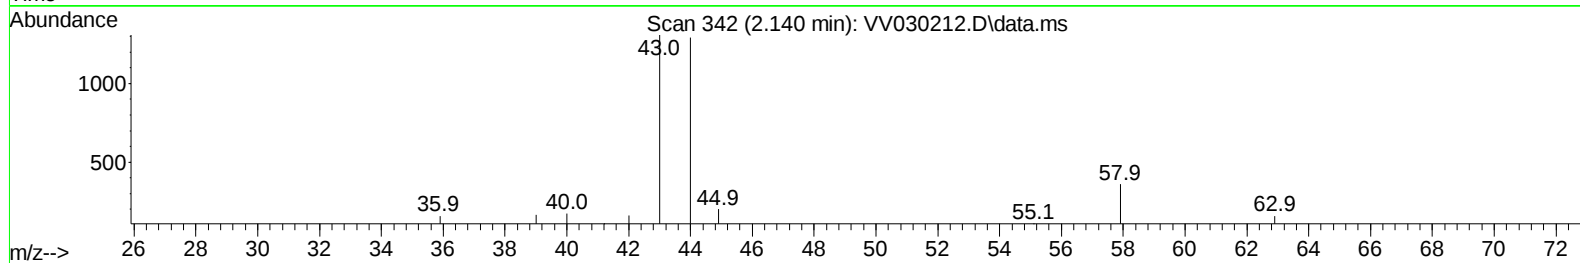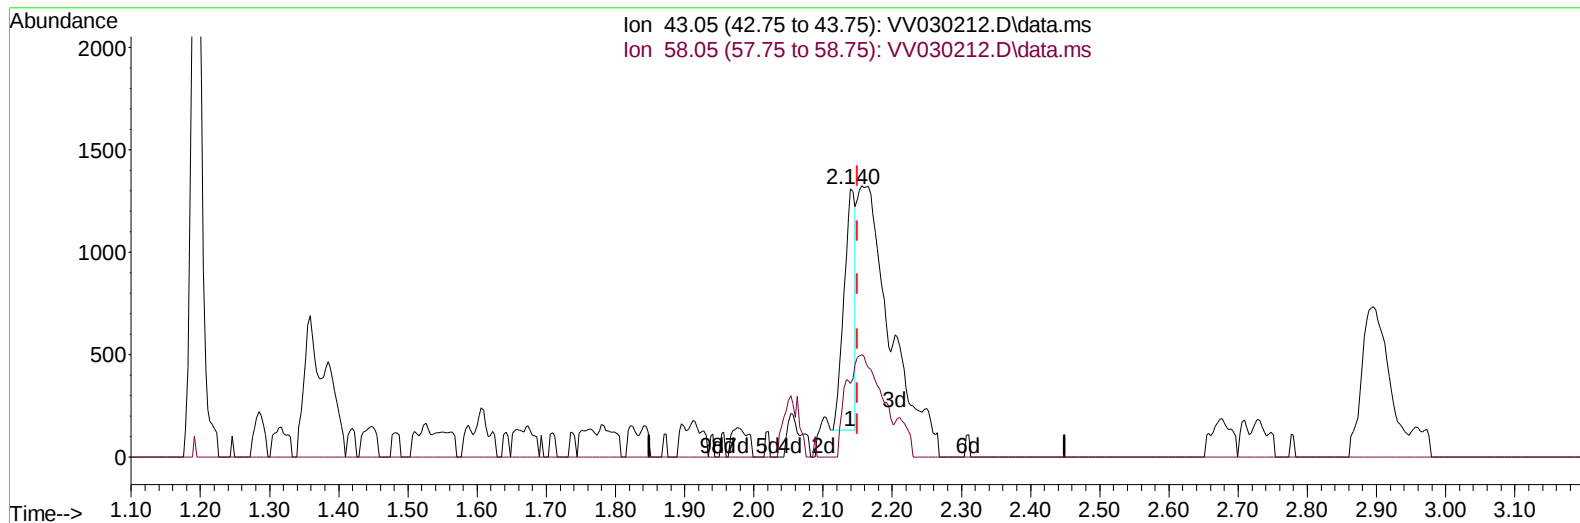

TIC: VV030212.D\data.ms

(13) Acetone (T)

2.140min (-0.010) 1.03 ug/L

response 1359

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	125.83#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030212.D
 Acq On : 15 Mar 2023 15:24
 Operator : SY/MD
 Sample : 01884-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB919

Manual IntegrationsAPPROVED

Quant Time: Mar 16 01:52:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 16 01:47:11 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

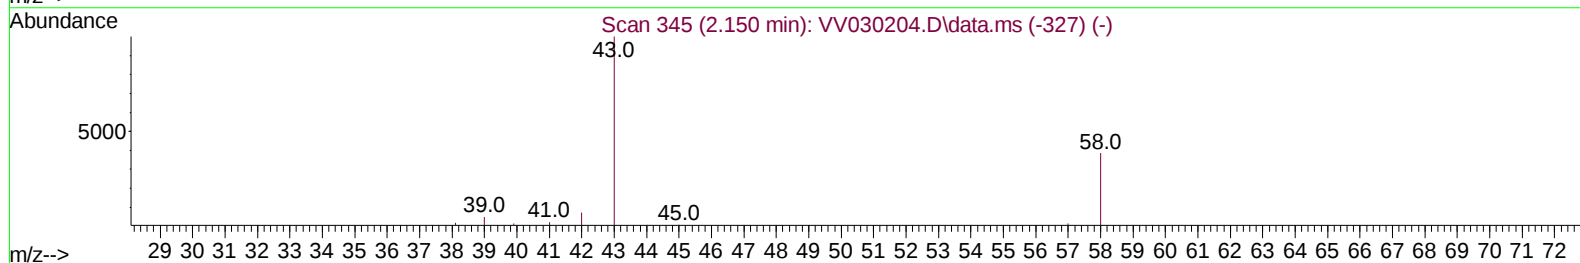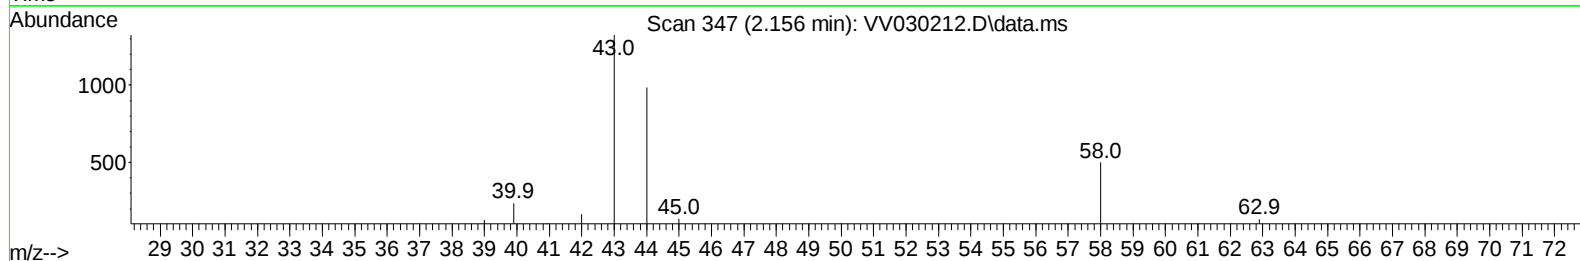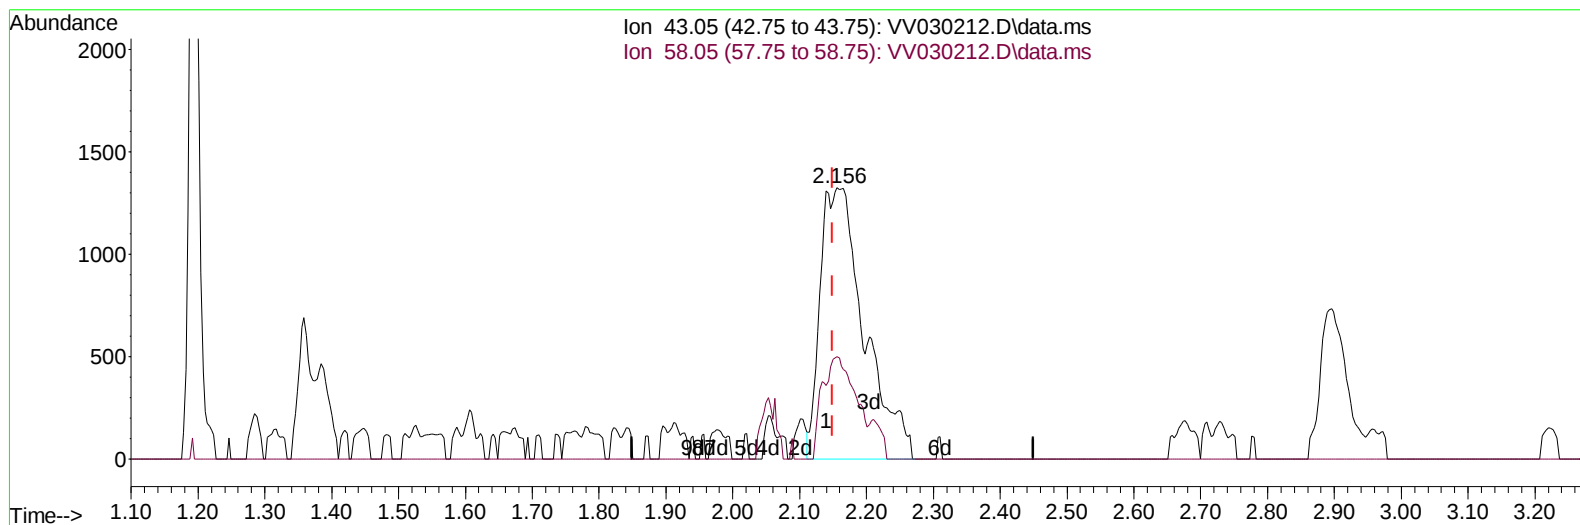

TIC: VV030212.D\data.ms

(13) Acetone (T)

2.156min (+ 0.006) 4.60 ug/L m

response 6100

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	28.03
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030212.D
 Acq On : 15 Mar 2023 15:24
 Operator : SY/MD
 Sample : 01884-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB919

Manual IntegrationsAPPROVED

Quant Time: Mar 16 01:52:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 16 01:47:11 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		150313	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		147480	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		76977	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.281	65		48650	5.002	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.000%	
7) Chloroethane-d5	1.539	69		44097	4.830	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.600%	
11) 1,1-Dichloroethene-d2	2.066	63		73107	3.656	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%	
20) 2-Butanone-d5	3.821	46		70266	39.185	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.380%	
24) Chloroform-d	4.259	84		95265	4.795	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%	
26) 1,2-Dichloroethane-d4	4.953	65		39581	4.880	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.600%	
32) Benzene-d6	4.973	84		179630	4.527	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%	
36) 1,2-Dichloropropane-d6	5.998	67		55951	4.687	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.800%	
41) Toluene-d8	7.252	98		153322	4.076	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.600%	
43) trans-1,3-Dichloroprop...	7.561	79		18450	4.517	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.037	63		63087	37.334	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.660%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		39378	4.636	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.800%	
66) 1,2-Dichlorobenzene-d4	11.570	152		63775	4.897	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.000%	
Target Compounds							
13) Acetone	2.156	43		6100m	4.603	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030212.D
Acq On : 15 Mar 2023 15:24
Operator : SY/MD
Sample : 01884-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
CB919

Manual IntegrationsAPPROVED

Quant Time: Mar 16 01:52:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 16 01:47:11 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
Supervised By :Mahesh Dadoda 03/17/2023

