

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030205.D
 Acq On : 15 Mar 2023 12:07
 Operator : SY/MD
 Sample : VV0315WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK312

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	66	rBV2	3212	4599	1.02%	0.121%
2	1.282	69	75	92	rVB	74951	81676	18.08%	2.150%
3	1.539	146	155	167	rVB	69136	80175	17.75%	2.111%
4	2.066	308	319	335	rBV	141621	207559	45.94%	5.465%
5	2.458	432	441	452	rVB4	3777	5748	1.27%	0.151%
6	3.828	855	867	908	rBV2	30314	131790	29.17%	3.470%
7	4.262	984	1002	1032	rBV2	82604	212791	47.10%	5.602%
8	4.969	1205	1222	1254	rBV2	174593	451775	100.00%	11.894%
9	5.545	1386	1401	1424	rBV	151975	311595	68.97%	8.204%
10	5.998	1529	1542	1562	rBV2	105744	218561	48.38%	5.754%
11	6.921	1817	1829	1853	rBV2	44000	83874	18.57%	2.208%
12	7.252	1919	1932	1952	rBV	206875	367287	81.30%	9.670%
13	7.564	2019	2029	2044	rBV	27761	49421	10.94%	1.301%
14	8.037	2165	2176	2210	rBV	173174	341579	75.61%	8.993%
15	8.792	2399	2411	2435	rBV	233879	393575	87.12%	10.362%
16	10.162	2823	2837	2853	rBV	84219	133753	29.61%	3.521%
17	11.194	3144	3158	3176	rBV	242988	383296	84.84%	10.091%
18	11.570	3263	3275	3293	rBV	213013	330125	73.07%	8.692%
19	12.207	3462	3473	3483	rVB2	5706	9059	2.01%	0.239%




Sum of corrected areas: 3798238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030205.D
Acq On : 15 Mar 2023 12:07
Operator : SY/MD
Sample : VV0315WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

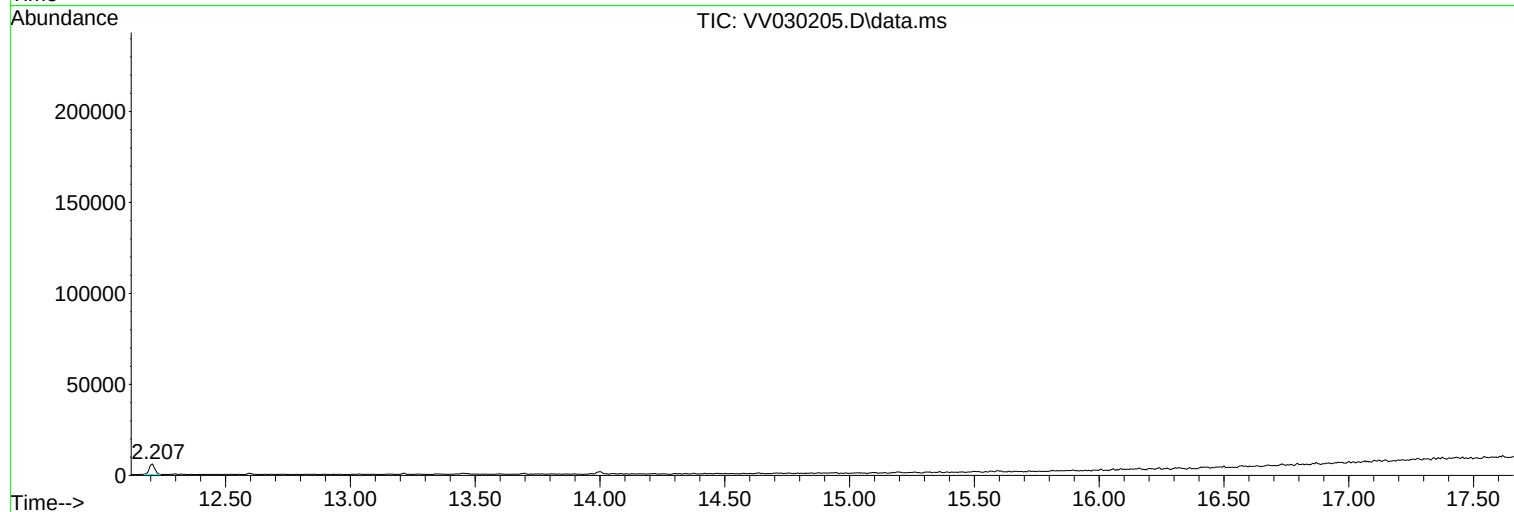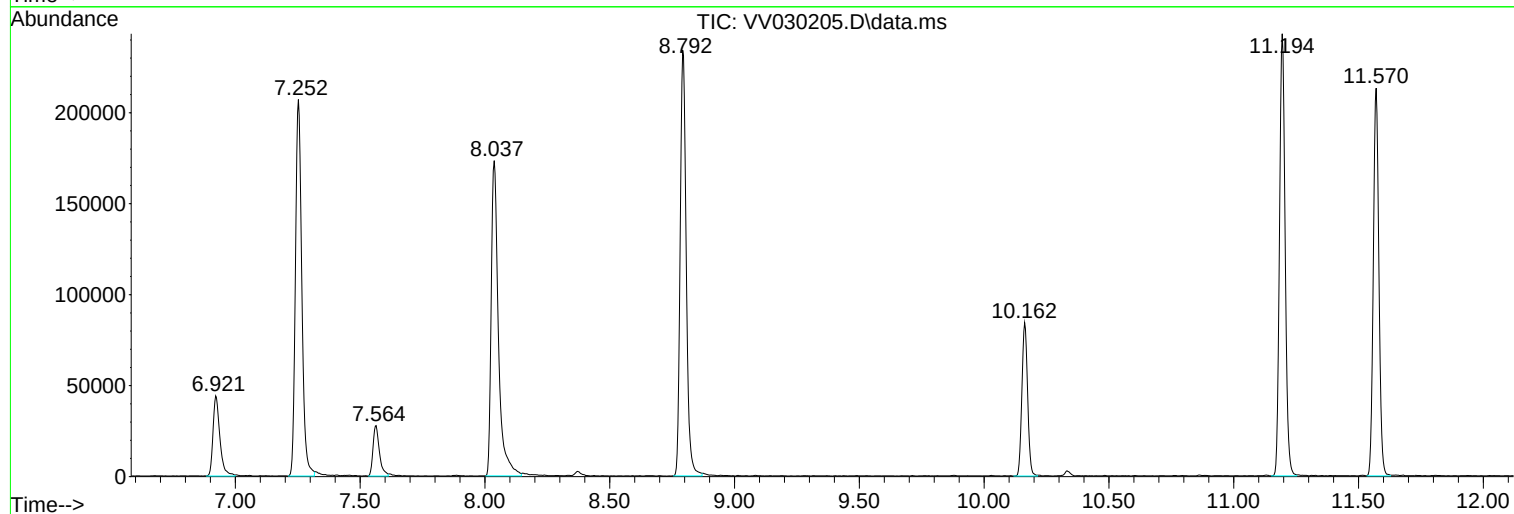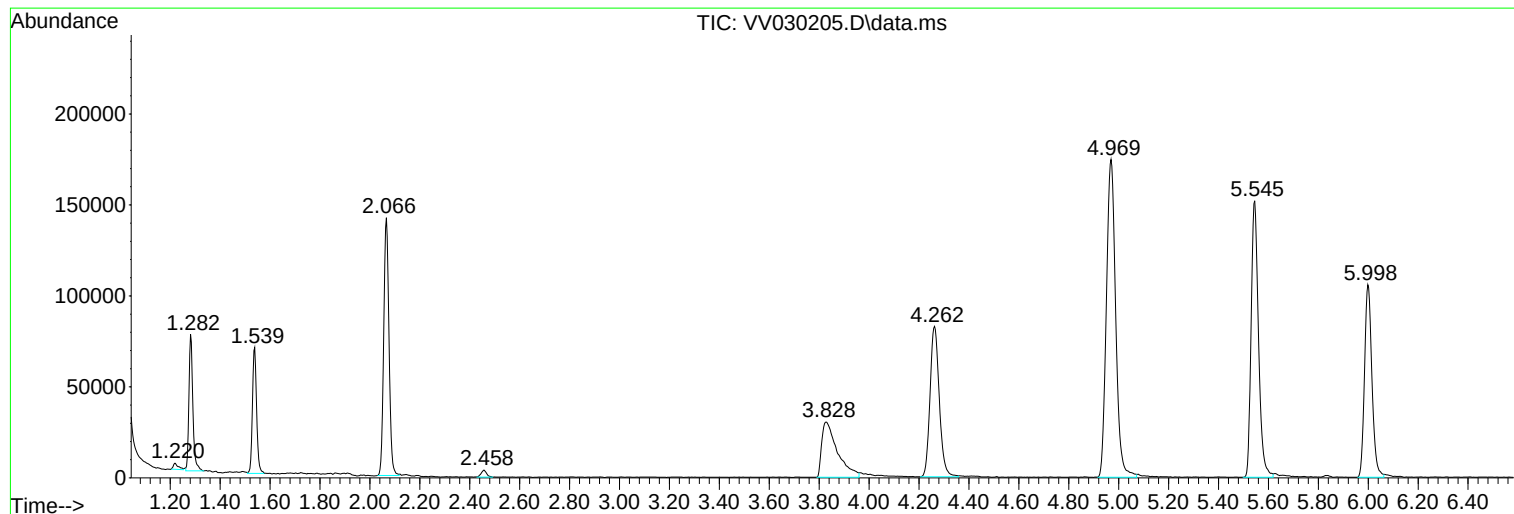

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030205.D
Acq On : 15 Mar 2023 12:07
Operator : SY/MD
Sample : VV0315WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030205.D
Acq On : 15 Mar 2023 12:07
Operator : SY/MD
Sample : VV0315WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc