

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030208.D
 Acq On : 15 Mar 2023 13:48
 Operator : SY/MD
 Sample : 01884-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB921

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	68	rBV	10795	14495	3.34%	0.340%
2	1.281	69	75	98	rVB	72208	84503	19.48%	1.983%
3	1.539	147	155	169	rVB	64146	75960	17.51%	1.782%
4	2.066	309	319	333	rBV	136125	199146	45.91%	4.673%
5	3.828	853	867	916	rBV2	99907	310407	71.56%	7.283%
6	4.262	985	1002	1023	rBV	80940	205037	47.27%	4.811%
7	4.969	1203	1222	1253	rBV2	169535	433792	100.00%	10.178%
8	5.545	1387	1401	1424	rBV	158927	324217	74.74%	7.607%
9	5.844	1482	1494	1518	rBV2	47733	97455	22.47%	2.287%
10	5.998	1529	1542	1571	rBV2	101316	211923	48.85%	4.972%
11	6.921	1818	1829	1855	rBV	44011	82374	18.99%	1.933%
12	7.252	1915	1932	1965	rBV	199575	358783	82.71%	8.418%
13	7.564	2019	2029	2045	rBV	26162	47006	10.84%	1.103%
14	7.886	2116	2129	2147	rVB	23270	43076	9.93%	1.011%
15	8.037	2166	2176	2205	rBV	167824	325685	75.08%	7.642%
16	8.792	2399	2411	2446	rBV	243980	415644	95.82%	9.752%
17	10.162	2825	2837	2856	rBV	80993	127790	29.46%	2.998%
18	10.336	2878	2891	2904	rVB	65748	110994	25.59%	2.604%
19	11.194	3147	3158	3178	rBV	261191	407802	94.01%	9.568%
20	11.497	3244	3252	3263	rBV3	8010	14584	3.36%	0.342%
21	11.570	3263	3275	3297	rVB	210793	334491	77.11%	7.848%
22	12.204	3460	3472	3484	rBV3	19136	30246	6.97%	0.710%
23	13.998	4021	4030	4042	rVB	4201	6621	1.53%	0.155%




Sum of corrected areas: 4262031

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030208.D
Acq On : 15 Mar 2023 13:48
Operator : SY/MD
Sample : 01884-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

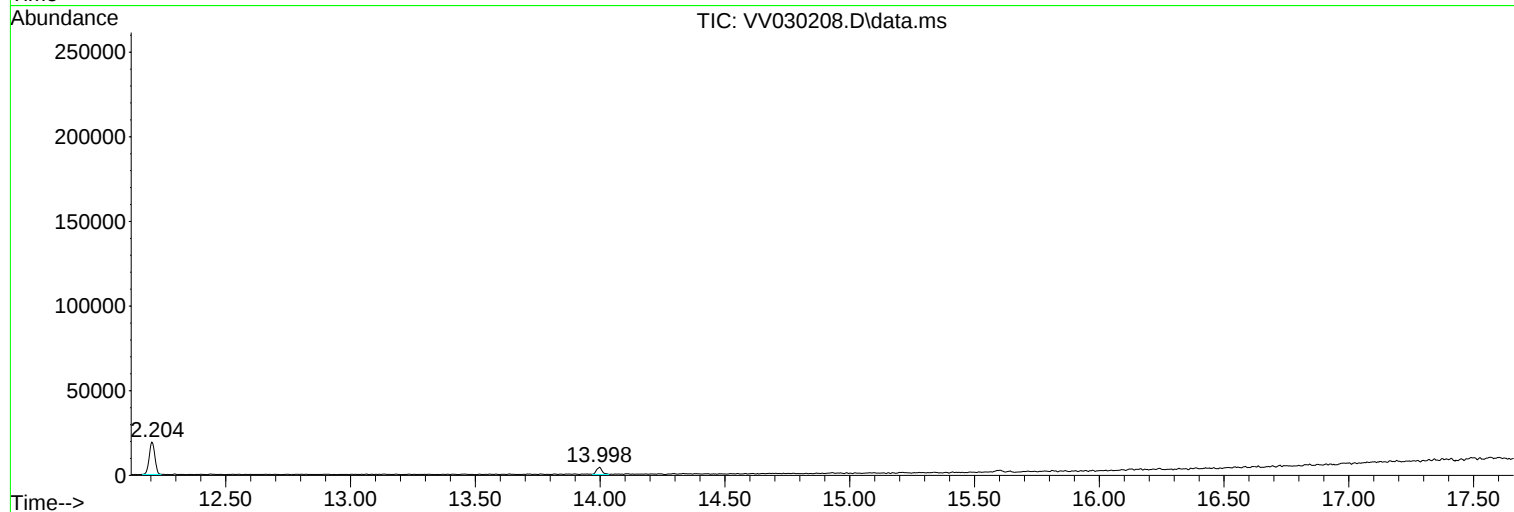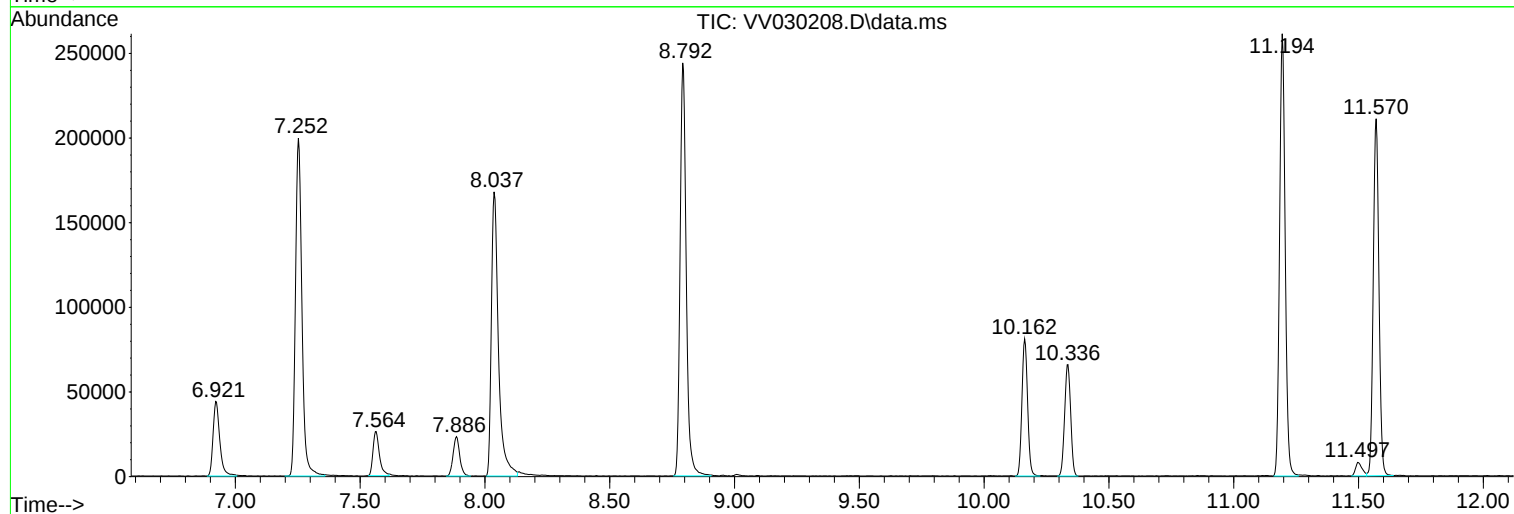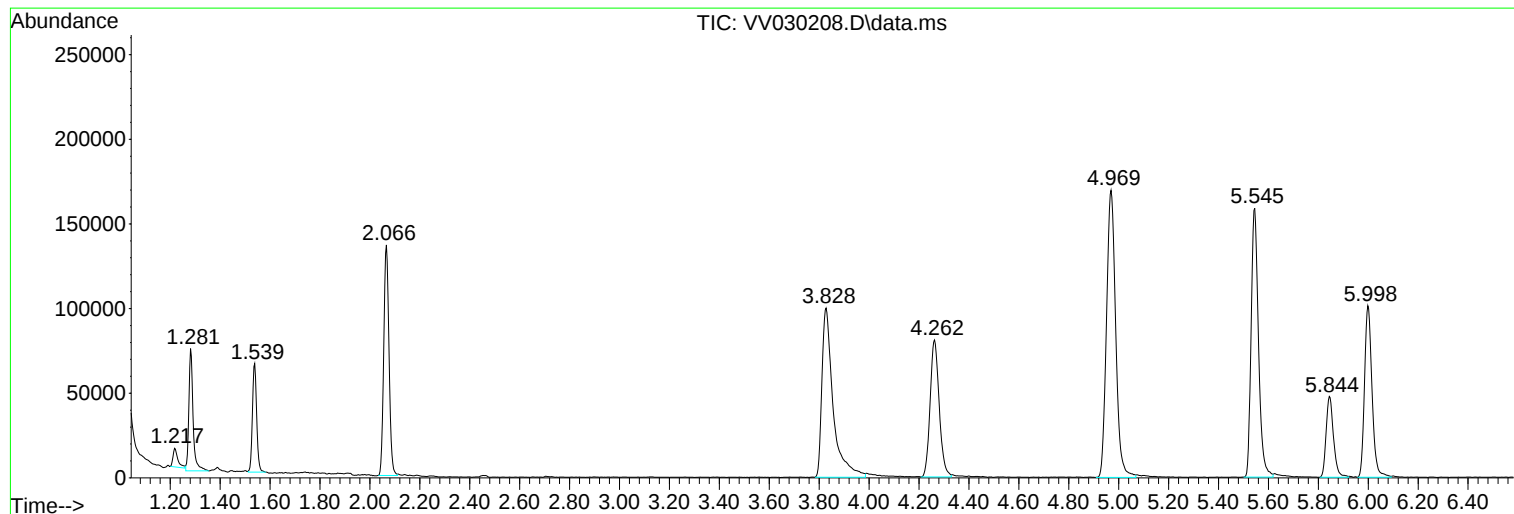

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030208.D
Acq On : 15 Mar 2023 13:48
Operator : SY/MD
Sample : 01884-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030208.D
Acq On : 15 Mar 2023 13:48
Operator : SY/MD
Sample : 01884-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------