

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030209.D
 Acq On : 15 Mar 2023 14:11
 Operator : SY/MD
 Sample : 01884-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB923

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	66	rVV	8045	9708	2.23%	0.255%
2	1.282	69	75	92	rVB	72829	81767	18.81%	2.146%
3	1.539	147	155	169	rVB	65559	77301	17.79%	2.028%
4	2.066	308	319	337	rBV	133349	194215	44.69%	5.096%
5	3.822	854	865	904	rBV	34509	129418	29.78%	3.396%
6	4.262	984	1002	1028	rBV2	81300	207953	47.85%	5.457%
7	4.970	1205	1222	1251	rBV2	169445	434625	100.00%	11.405%
8	5.545	1388	1401	1422	rBV	148529	309438	71.20%	8.120%
9	5.998	1529	1542	1567	rBV	98952	210127	48.35%	5.514%
10	6.924	1819	1830	1854	rBV	42862	81317	18.71%	2.134%
11	7.252	1917	1932	1964	rBV	201035	361751	83.23%	9.493%
12	7.561	2019	2028	2045	rBV	26586	47396	10.91%	1.244%
13	7.886	2113	2129	2143	rBV	10633	19828	4.56%	0.520%
14	8.037	2165	2176	2208	rBV	171821	332439	76.49%	8.724%
15	8.793	2399	2411	2444	rBV	233144	395334	90.96%	10.374%
16	10.162	2822	2837	2854	rBV	82260	130401	30.00%	3.422%
17	10.333	2879	2890	2903	rVB2	33994	55065	12.67%	1.445%
18	11.194	3147	3158	3179	rBV	246695	385025	88.59%	10.103%
19	11.571	3263	3275	3293	rVV	214040	330479	76.04%	8.672%
20	12.204	3460	3472	3483	rBV2	10461	17222	3.96%	0.452%




Sum of corrected areas: 3810809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030209.D
Acq On : 15 Mar 2023 14:11
Operator : SY/MD
Sample : 01884-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

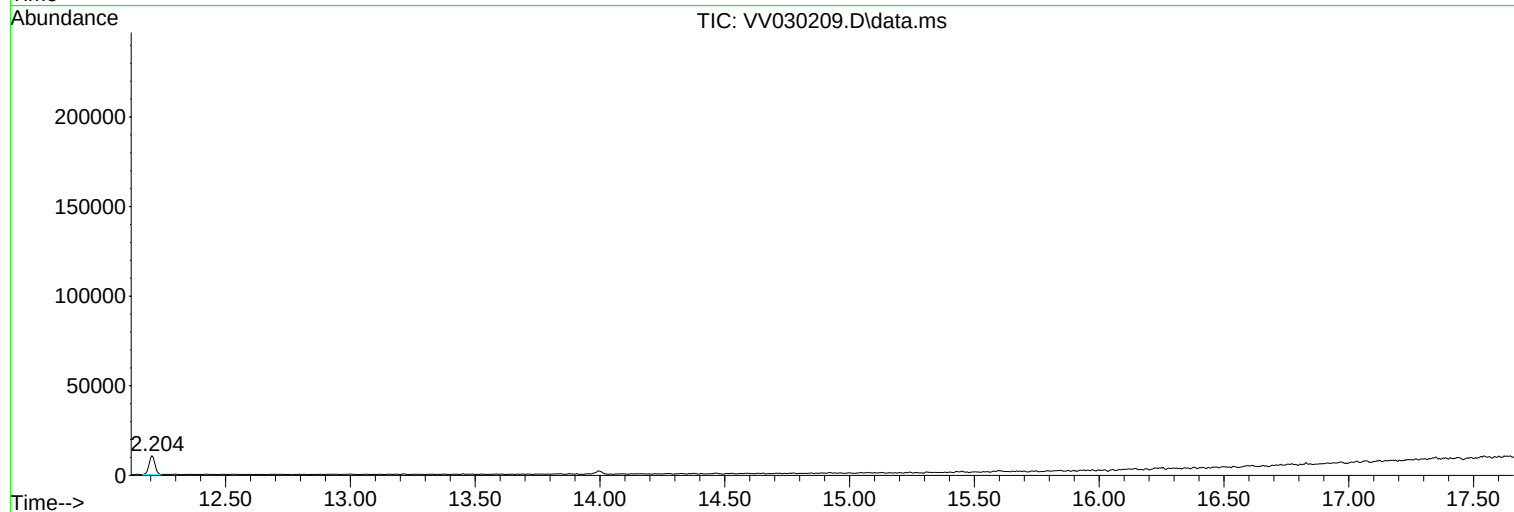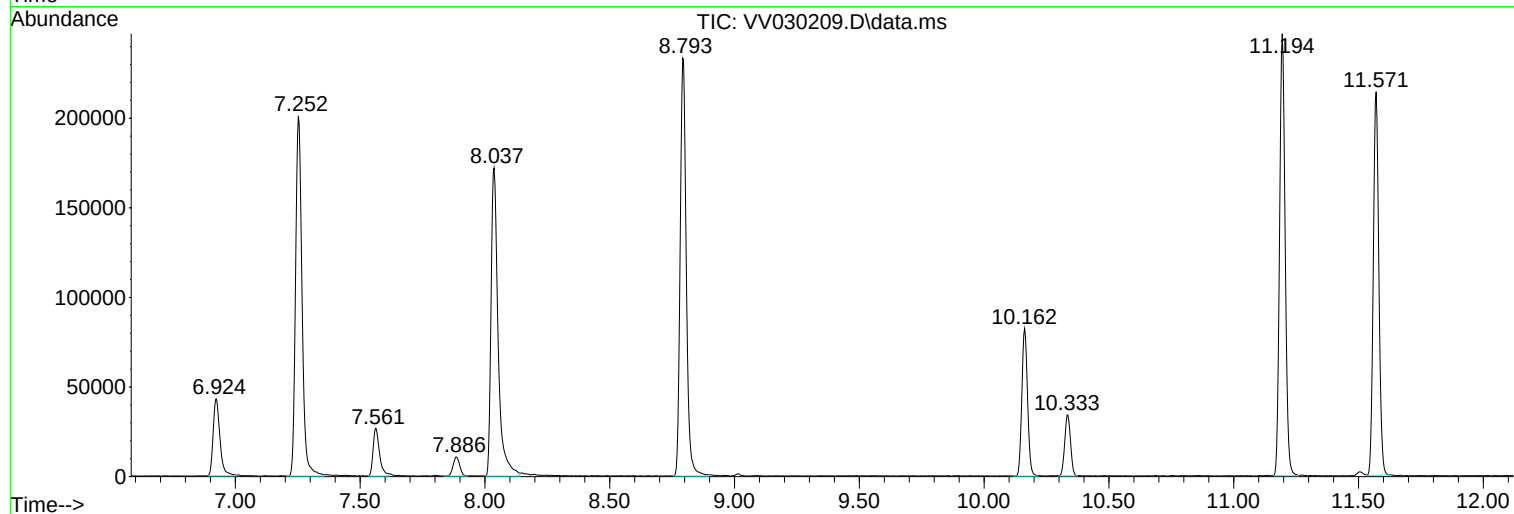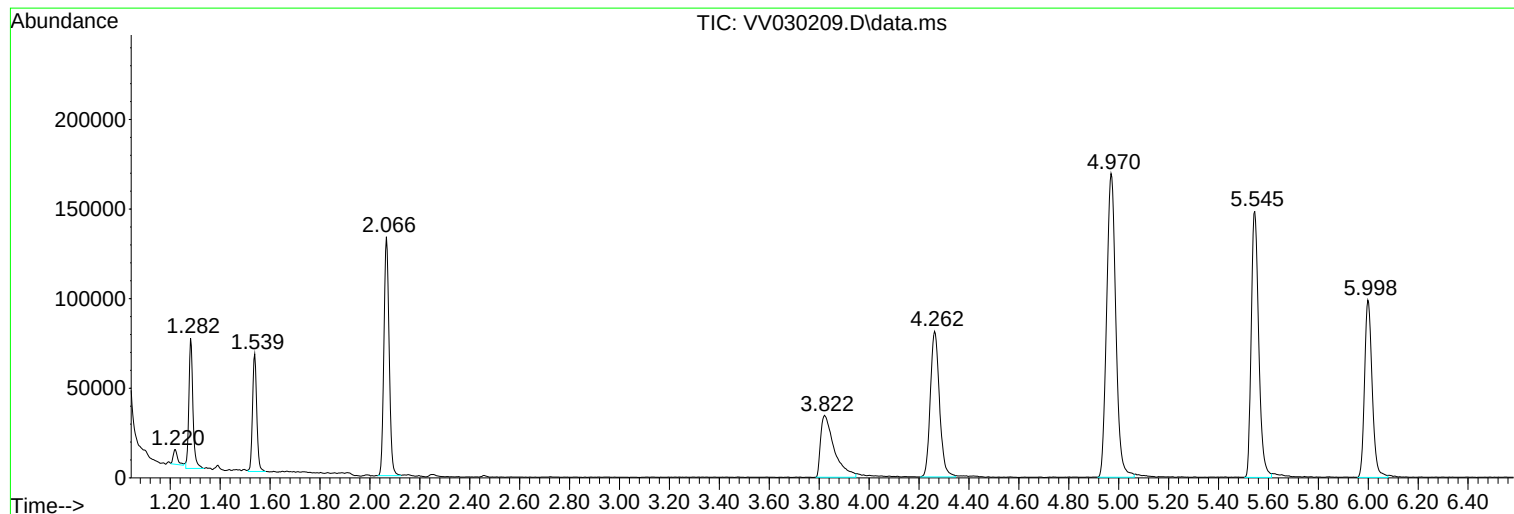

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030209.D
Acq On : 15 Mar 2023 14:11
Operator : SY/MD
Sample : 01884-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030209.D
Acq On : 15 Mar 2023 14:11
Operator : SY/MD
Sample : 01884-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------