

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030214.D
 Acq On : 15 Mar 2023 16:12
 Operator : SY/MD
 Sample : VIBLK280
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK280

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	94	rVB	79023	87607	17.42%	1.969%
2	1.539	147	155	167	rVB	72869	86909	17.28%	1.953%
3	2.066	306	319	340	rBV	149923	219989	43.73%	4.943%
4	2.455	431	440	453	rVB2	5593	9625	1.91%	0.216%
5	3.818	851	864	903	rBV	43833	164168	32.64%	3.689%
6	4.259	985	1001	1027	rBV	89679	229948	45.71%	5.167%
7	4.969	1205	1222	1248	rBV2	197779	503039	100.00%	11.303%
8	5.545	1387	1401	1429	rBV	188824	396219	78.77%	8.903%
9	5.998	1529	1542	1575	rBV	114208	237595	47.23%	5.339%
10	6.921	1819	1829	1860	rBV2	49553	94089	18.70%	2.114%
11	7.252	1920	1932	1967	rBV	240728	430213	85.52%	9.667%
12	7.564	2018	2029	2049	rBV	30427	54820	10.90%	1.232%
13	8.037	2164	2176	2204	rBV	207801	385160	76.57%	8.655%
14	8.368	2269	2279	2291	rBV3	9814	17412	3.46%	0.391%
15	8.792	2400	2411	2439	rBV	291213	489459	97.30%	10.998%
16	10.162	2826	2837	2856	rBV	90789	145339	28.89%	3.266%
17	10.336	2880	2891	2902	rBV2	4934	7575	1.51%	0.170%
18	11.194	3145	3158	3177	rBV	313916	483736	96.16%	10.870%
19	11.570	3263	3275	3290	rBV	243682	387333	77.00%	8.703%
20	12.207	3460	3473	3482	rBV	7353	11228	2.23%	0.252%
21	16.435	4780	4788	4795	rVB2	6345	8922	1.77%	0.200%




Sum of corrected areas: 4450385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030214.D
Acq On : 15 Mar 2023 16:12
Operator : SY/MD
Sample : VIBLK280
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

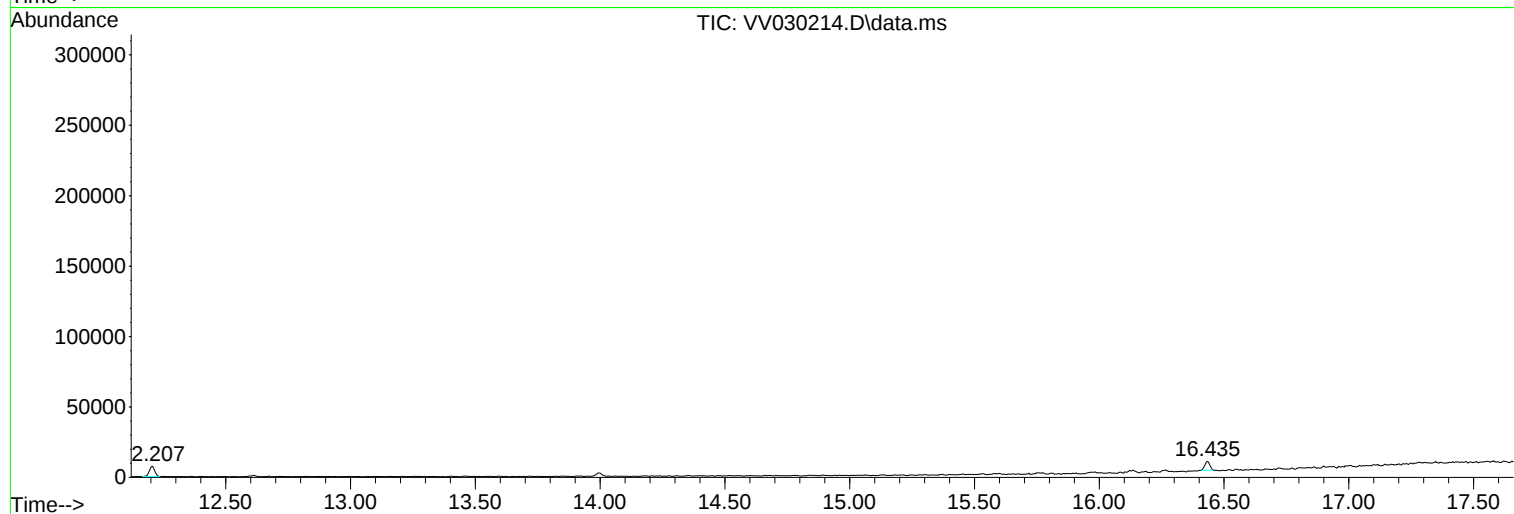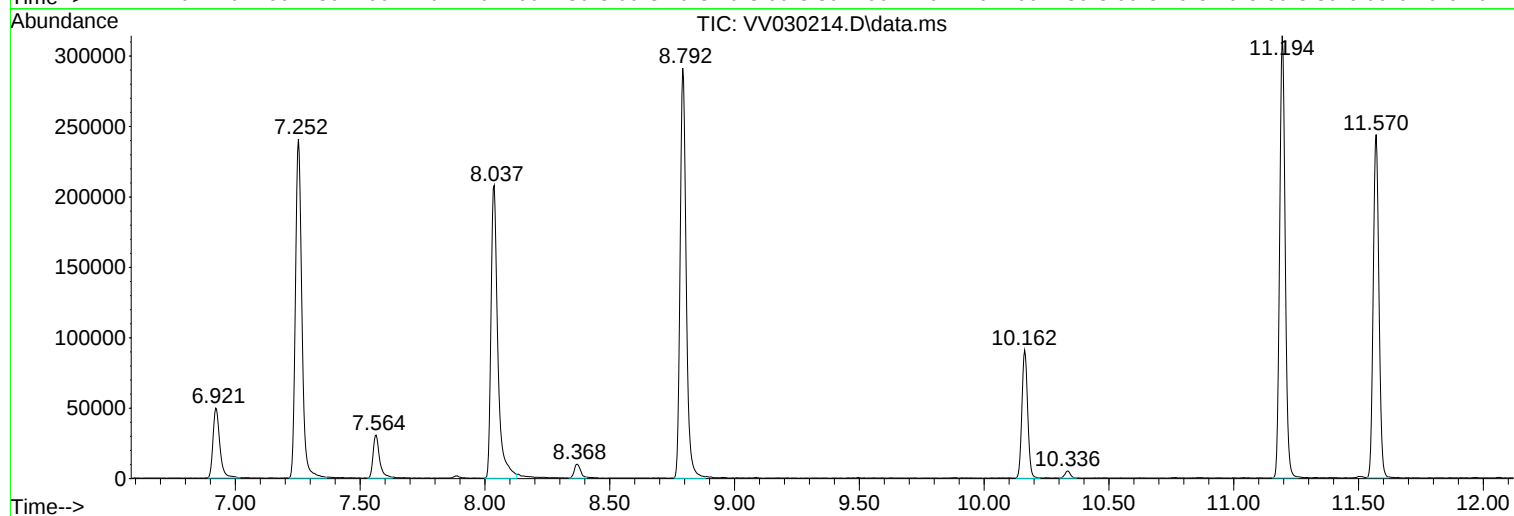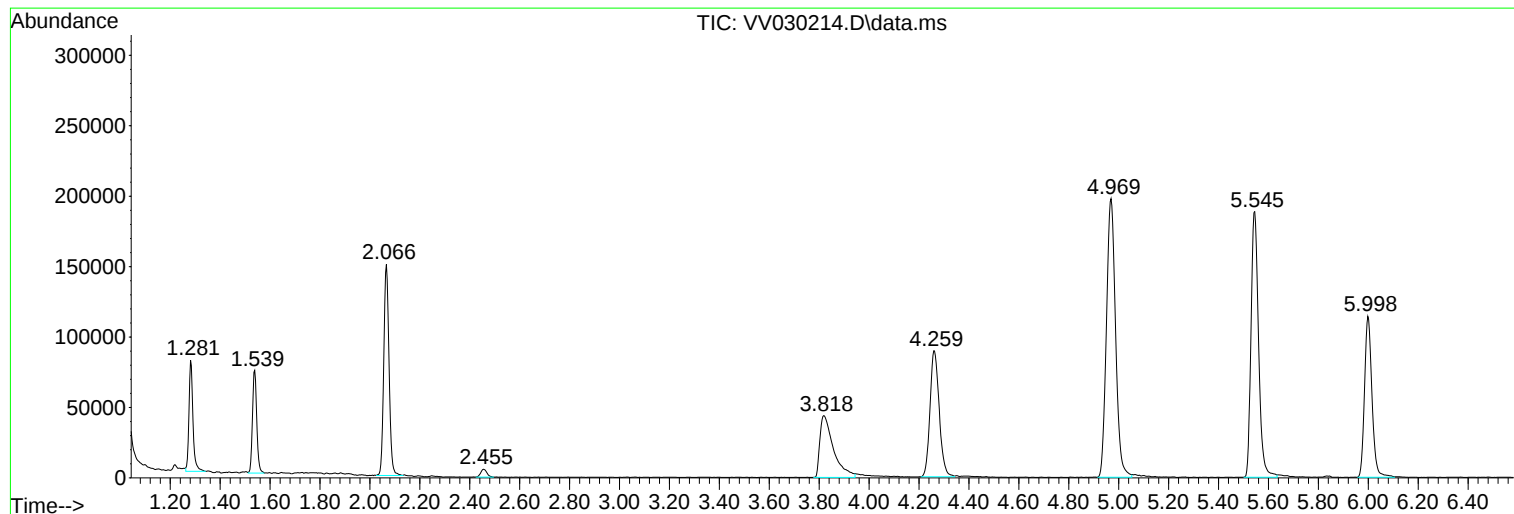

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030214.D
Acq On : 15 Mar 2023 16:12
Operator : SY/MD
Sample : VIBLK280
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
Data File : VV030214.D
Acq On : 15 Mar 2023 16:12
Operator : SY/MD
Sample : VIBLK280
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------