


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031523\
 Data File : VV030203.D
 Acq On : 15 Mar 2023 10:44
 Operator : SY/MD
 Sample : BFB232
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB232

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 17 05:46:57 2023

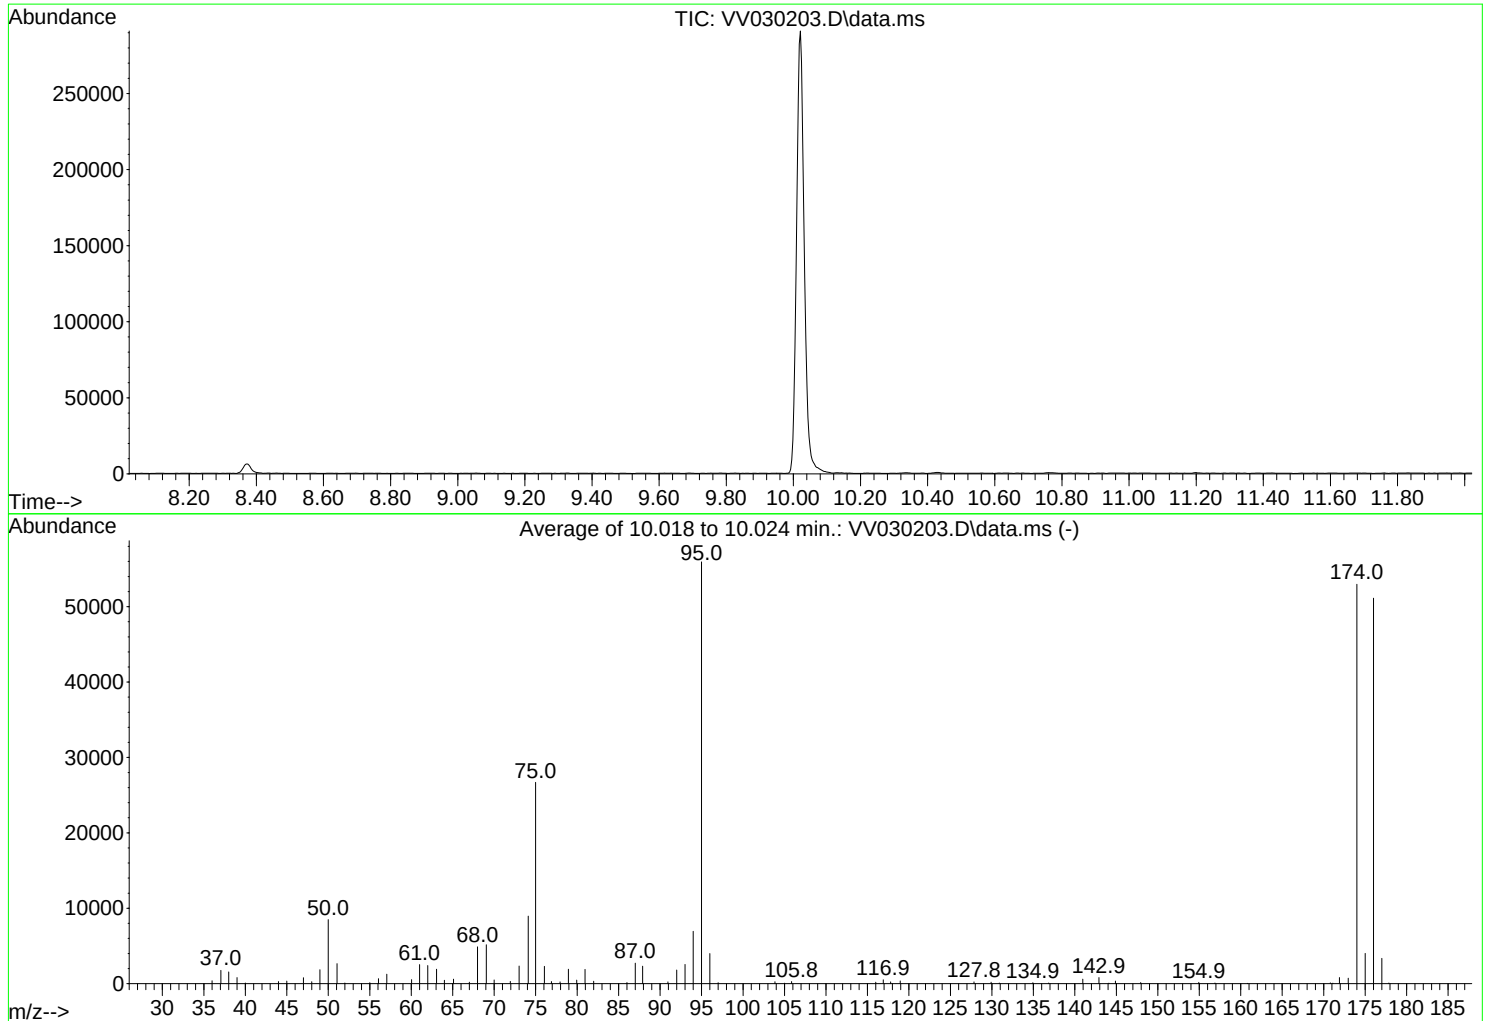

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	8493	PASS
75	95	30	80	47.7	26696	PASS
95	95	100	100	100.0	55947	PASS
96	95	5	9	7.1	3988	PASS
173	174	0.00	2	1.4	720	PASS
174	95	50	120	94.7	52981	PASS
175	174	5	9	7.6	4012	PASS
176	174	95	105	96.5	51136	PASS
177	176	5	10	6.6	3350	PASS

m/z	Abundance
40.00	148.0
44.00	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	400.0
37.10	1864.0
38.00	1528.0
39.00	867.0
40.00	245.0
44.00	468.0
45.00	324.0
47.00	818.0
48.00	294.0
49.00	1961.0
50.00	8592.0
51.10	2638.0
52.00	140.0
55.00	127.0
56.10	743.0
57.10	1311.0
60.00	491.0
61.00	2540.0
62.00	2436.0
63.00	1968.0
64.00	388.0
65.10	577.0
67.00	183.0
68.00	5078.0
69.10	5232.0
70.00	439.0
71.90	279.0
73.00	2336.0
74.10	9005.0
75.00	27264.0
76.10	2305.0
76.90	309.0
78.00	227.0
78.90	1936.0
79.90	449.0
81.00	1882.0
82.00	355.0
86.00	167.0
87.00	2786.0
87.90	2485.0
90.90	240.0
92.00	1837.0
93.00	2399.0
94.00	6965.0
95.00	56632.0
96.00	4022.0
97.00	126.0
103.90	263.0
105.90	309.0
116.00	156.0
116.90	494.0
117.80	244.0
119.00	409.0
127.80	262.0
129.90	201.0
130.90	151.0
135.00	119.0
136.90	120.0
140.90	624.0
142.90	830.0
144.90	318.0
147.90	168.0
154.90	162.0
156.90	122.0
160.80	106.0
171.10	166.0
171.90	781.0
172.90	760.0
174.00	52336.0
175.00	4132.0
176.00	50336.0
177.00	3204.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	398.0
37.10	1808.0
38.00	1619.0
39.00	823.0
40.00	229.0
44.00	489.0
45.00	354.0
47.00	824.0
48.00	280.0
49.00	1908.0
50.00	8813.0
51.00	2718.0
52.00	104.0
55.00	142.0
56.10	674.0
57.00	1268.0
60.00	545.0
61.00	2613.0
62.00	2524.0
63.10	1957.0
64.00	482.0
65.10	623.0
67.00	209.0
68.00	5074.0
69.00	5267.0
70.00	525.0
72.00	299.0
73.00	2418.0
74.10	9317.0
75.00	27672.0
76.00	2351.0
76.90	291.0
78.00	268.0
78.90	1950.0
79.90	483.0
81.00	1973.0
82.00	331.0
86.00	168.0
87.00	2832.0
87.90	2434.0
91.00	231.0
92.00	1883.0
93.00	2656.0
94.00	7124.0
95.00	57664.0
96.00	4131.0
97.00	146.0
103.80	251.0
105.00	105.0
105.80	296.0
116.00	197.0
116.90	518.0
117.80	254.0
119.00	374.0
127.90	243.0
129.90	203.0
130.90	105.0
135.00	152.0
136.80	112.0
140.90	611.0
142.90	808.0
144.10	112.0
144.90	364.0
148.00	155.0
155.00	164.0
156.90	109.0
170.80	181.0
171.90	856.0
173.00	727.0
174.00	54840.0
175.00	4093.0
176.00	52800.0
177.00	3484.0
177.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	336.0
37.00	1614.0
38.00	1480.0
39.00	712.0
40.00	208.0
44.00	515.0
45.00	351.0
47.00	734.0
48.00	220.0
49.00	1688.0
50.00	8074.0
51.00	2578.0
55.00	146.0
56.00	530.0
57.00	1197.0
60.10	556.0
61.00	2407.0
62.00	2265.0
63.10	1796.0
64.00	469.0
65.10	594.0
67.00	197.0
68.00	4505.0
69.00	4983.0
70.00	511.0
72.00	297.0
73.00	2259.0
74.10	8523.0
75.00	25152.0
76.00	2212.0
76.90	234.0
77.90	234.0
79.00	1829.0
80.00	461.0
80.90	1828.0
82.00	283.0
86.00	132.0
87.00	2542.0
87.90	2037.0
91.00	204.0
92.00	1669.0
93.00	2584.0
94.00	6703.0
95.00	53544.0
96.00	3810.0
97.00	124.0
103.80	241.0
105.00	103.0
105.80	231.0
116.00	205.0
116.90	498.0
117.80	222.0
118.90	291.0
127.90	220.0
129.90	204.0
134.90	128.0
141.00	542.0
142.90	785.0
144.10	107.0
144.90	328.0
148.00	135.0
155.00	175.0
170.80	170.0
171.90	800.0
173.00	673.0
174.00	51768.0
175.00	3810.0
176.00	50272.0
177.00	3363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232