

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034666.D
 Acq On : 15 Mar 2024 20:41
 Operator : SY/MD
 Sample : P1740-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 16 01:14:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 16 00:58:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	349853	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	328749	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	151764	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	90277	29.766	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	59.540%#
7) Chloroethane-d5	1.532	69	84906	35.934	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	71.860%
11) 1,1-Dichloroethene-d2	2.060	65	45681	33.305	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.600%
21) 2-Butanone-d5	3.796	46	181851	89.662	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.660%
24) Chloroform-d	4.249	84	210010	39.163	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.320%
26) 1,2-Dichloroethane-d4	4.941	65	141683	40.432	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.860%
32) Benzene-d6	4.960	84	388381	39.144	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.280%
36) 1,2-Dichloropropane-d6	5.986	67	128252	42.356	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.720%
41) Toluene-d8	7.243	98	338143	37.661	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.320%#
43) trans-1,3-Dichloroprop...	7.555	79	55062	36.212	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.420%
47) 2-Hexanone-d5	8.024	63	129075	85.366	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.370%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	179687	45.094	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.180%
66) 1,2-Dichlorobenzene-d4	11.561	152	135162	43.571	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.140%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	11.185	75	18260	6.303	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034666.D
Acq On : 15 Mar 2024 20:41
Operator : SY/MD
Sample : P1740-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 16 01:14:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 16 00:58:04 2024
Response via : Initial Calibration

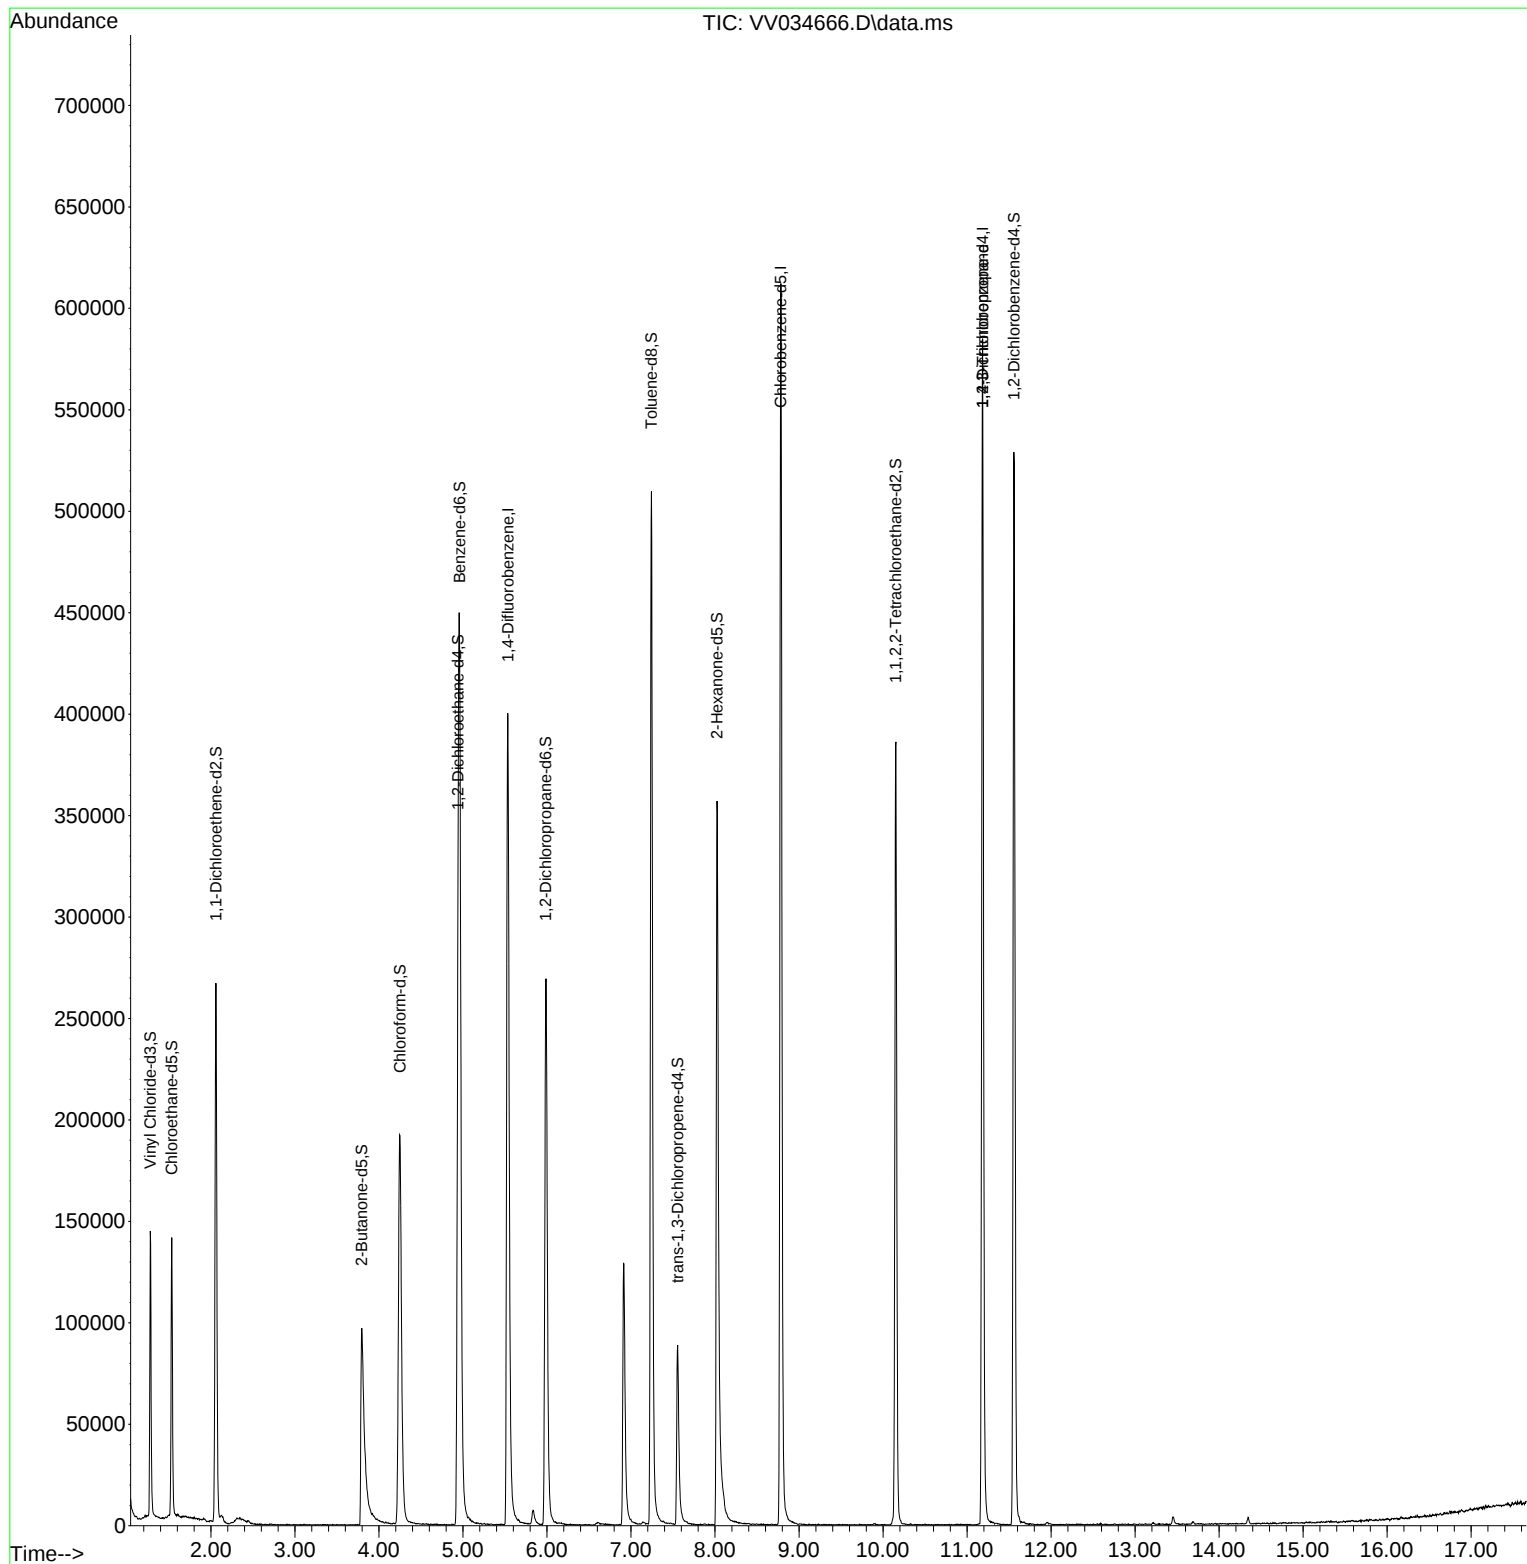

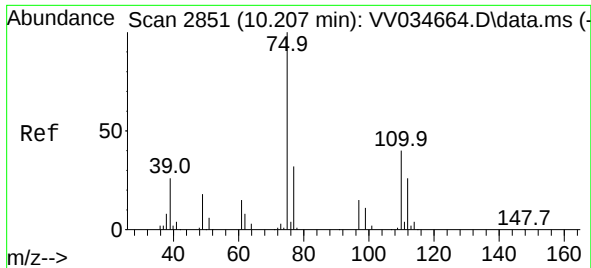

#61
 1,2,3-Trichloropropane
 Concen: 6.303 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.978 min
 Lab File: VV034666.D
 Acq: 15 Mar 2024 20:41

Instrument :
 MSVOA_V
 ClientSampleId :

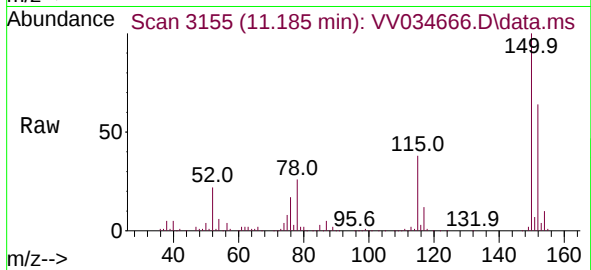

Tgt Ion: 75	Resp: 18260
Ion Ratio	Lower Upper
75	100
77	32.7 25.9 38.9
110	2.8 33.1 49.7#

