

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034671.D
 Acq On : 15 Mar 2024 22:40
 Operator : SY/MD
 Sample : P1740-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 16 01:15:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 16 00:58:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	344759	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	318387	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	146481	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	88923	29.753	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	59.500%#
7) Chloroethane-d5	1.529	69	85479	36.711	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	73.420%
11) 1,1-Dichloroethene-d2	2.056	65	44488	32.914	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.820%
21) 2-Butanone-d5	3.789	46	176316	88.217	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.220%
24) Chloroform-d	4.249	84	204752	38.747	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.500%
26) 1,2-Dichloroethane-d4	4.940	65	139940	40.525	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.040%
32) Benzene-d6	4.960	84	384769	40.043	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.080%
36) 1,2-Dichloropropane-d6	5.989	67	124588	42.486	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.980%
41) Toluene-d8	7.243	98	331300	38.099	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.200%#
43) trans-1,3-Dichloroprop...	7.555	79	52797	35.853	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.700%
47) 2-Hexanone-d5	8.024	63	123827	84.561	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.560%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	174594	45.242	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.480%
66) 1,2-Dichlorobenzene-d4	11.561	152	129097	43.117	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.240%
Target Compounds						
61) 1,2,3-Trichloropropane	11.185	75	17641	6.309	ug/L	Qvalue # 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034671.D
Acq On : 15 Mar 2024 22:40
Operator : SY/MD
Sample : P1740-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 16 01:15:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 16 00:58:04 2024
Response via : Initial Calibration

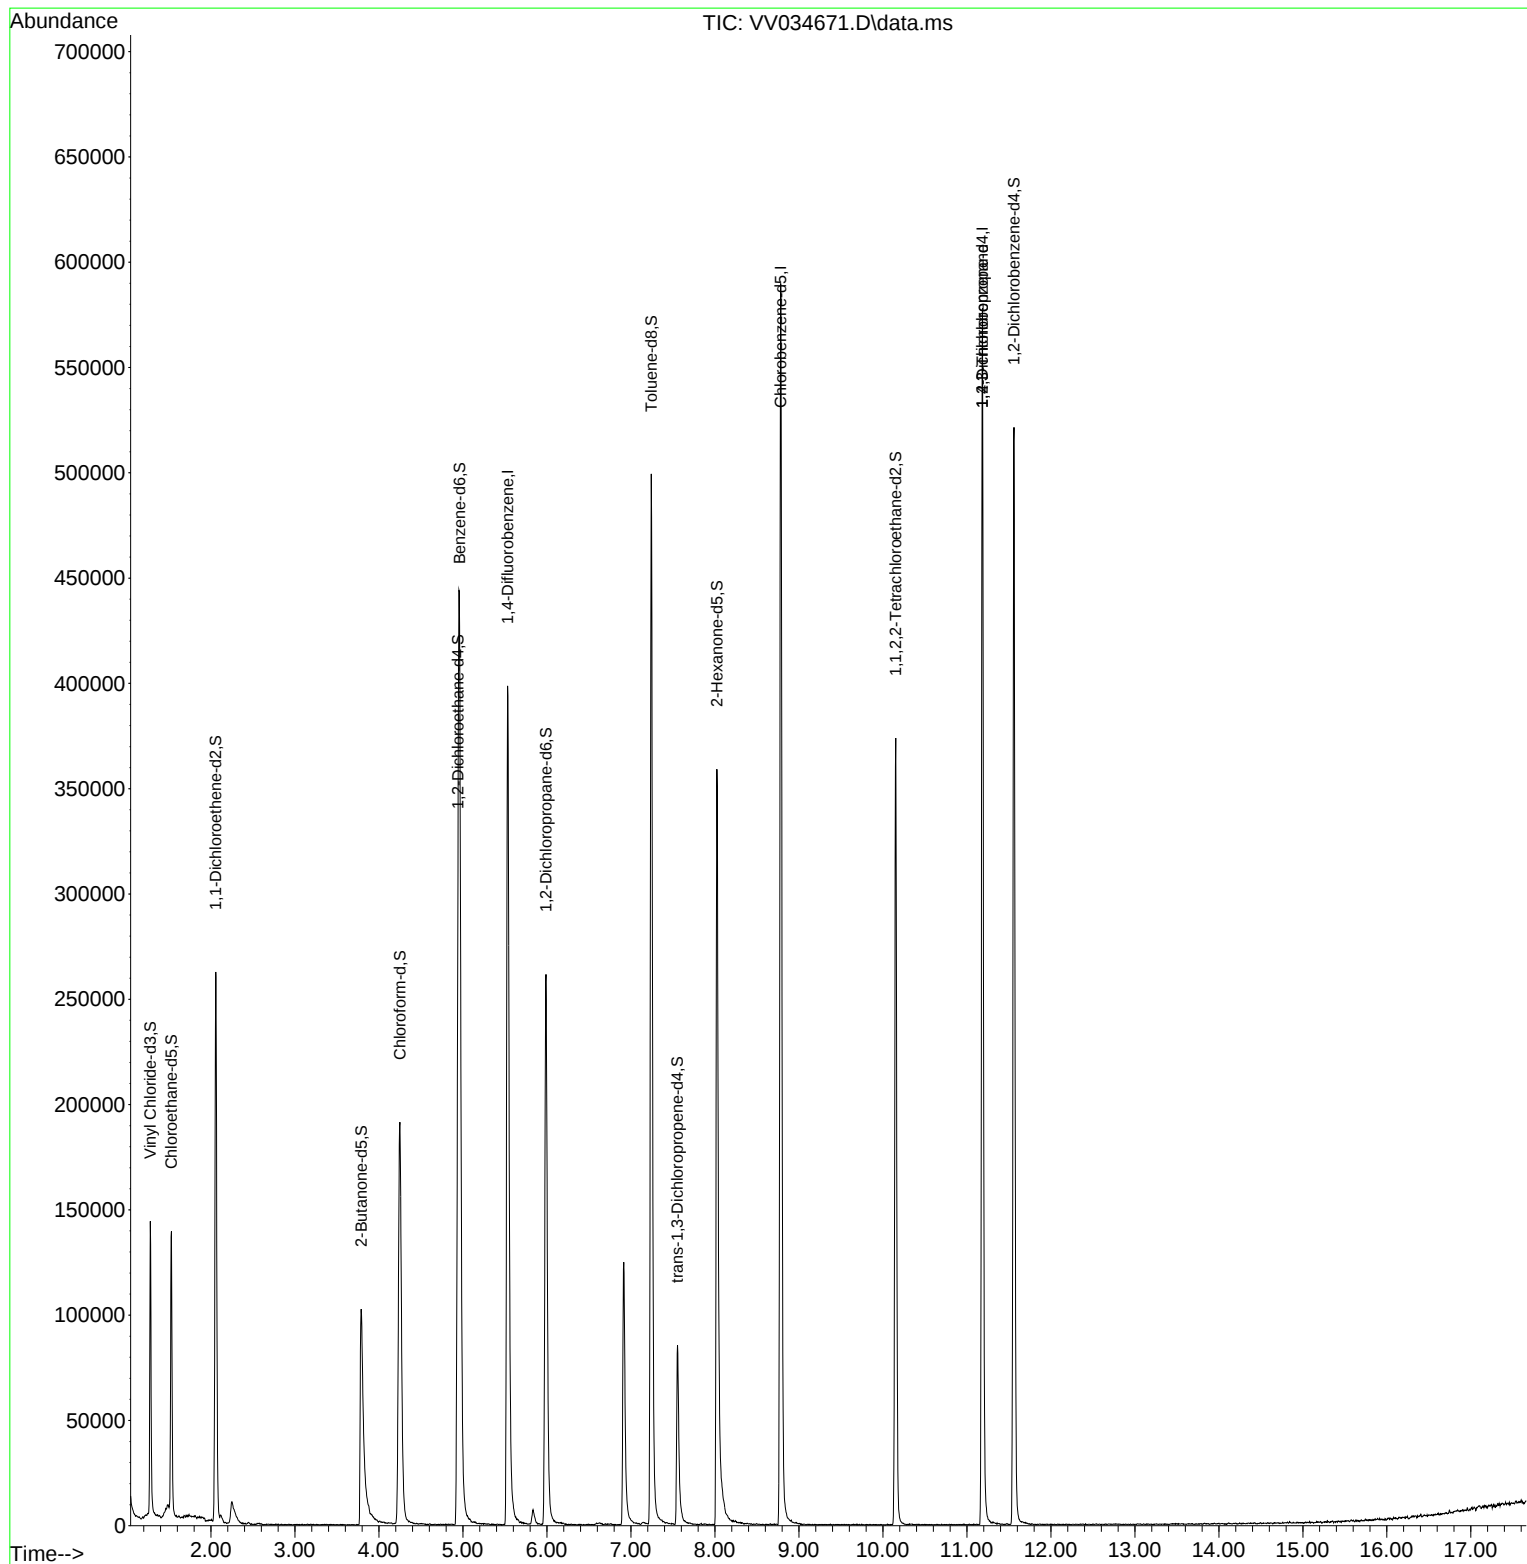

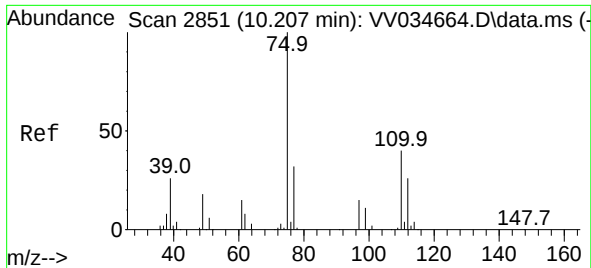

#61
 1,2,3-Trichloropropane
 Concen: 6.309 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.977 min
 Lab File: VV034671.D
 Acq: 15 Mar 2024 22:40

Instrument :
 MSVOA_V
 ClientSampleId :

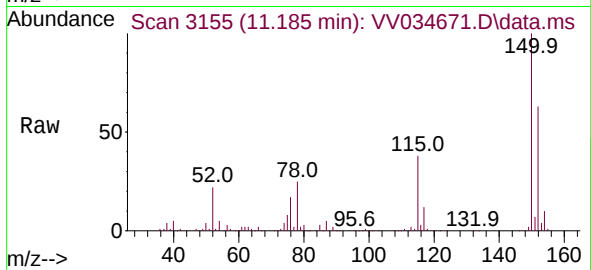

Tgt Ion:	75	Resp:	17641
Ion Ratio	Lower	Upper	
75	100		
77	33.4	25.9	38.9
110	2.2	33.1	49.7#

