




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034655.D
Acq On : 15 Mar 2024 15:54
Operator : SY/MD
Sample : P1752-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL31

Manual IntegrationsAPPROVED

Quant Time: Mar 15 23:35:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 23:30:32 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/19/2024
Supervised By :Semsettin Yesilyurt 03/19/2024

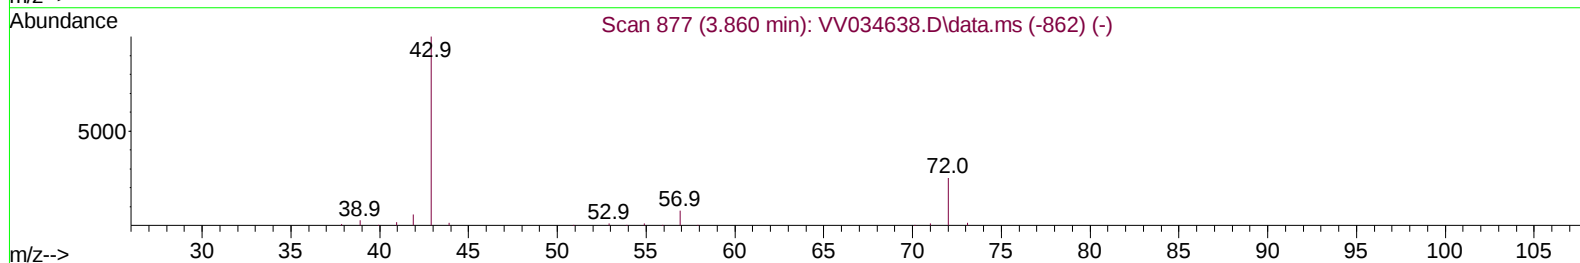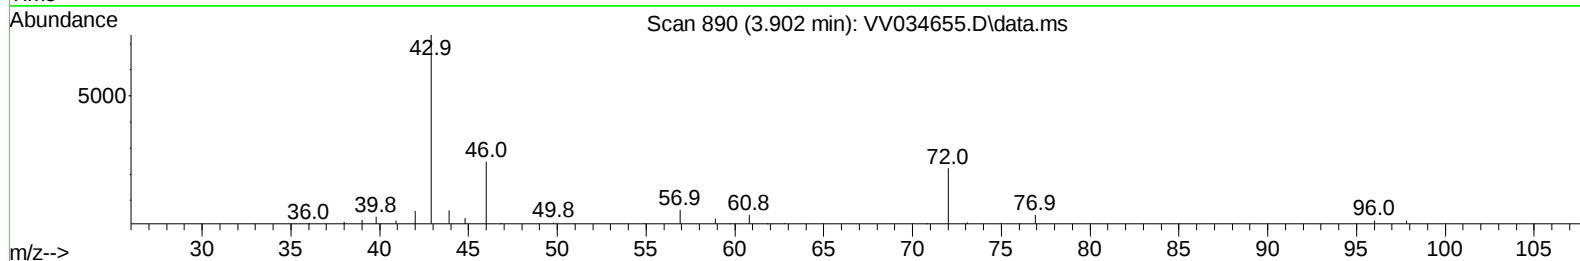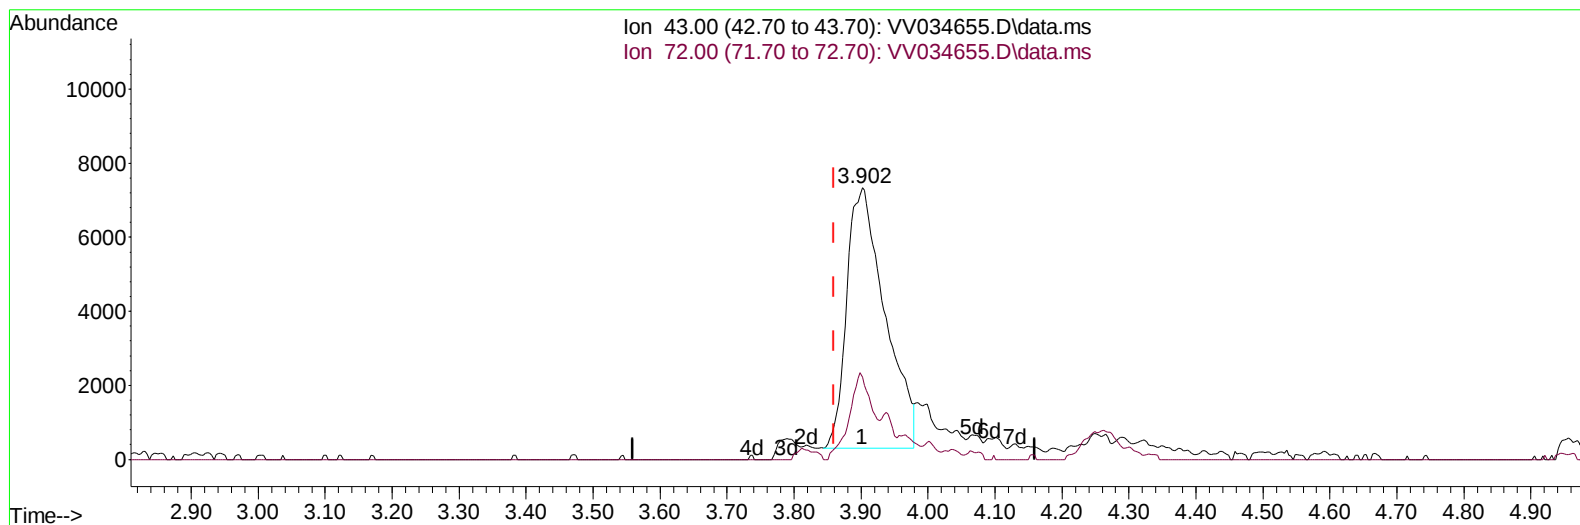

TIC: VV034655.D\data.ms

(22) 2-Butanone (T)

3.902min (+ 0.042) 11.94 ug/L

response 27904

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	22.90	19.94
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034655.D
Acq On : 15 Mar 2024 15:54
Operator : SY/MD
Sample : P1752-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL31

Manual IntegrationsAPPROVED

Quant Time: Mar 15 23:35:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 23:30:32 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/19/2024
Supervised By :Semsettin Yesilyurt 03/19/2024

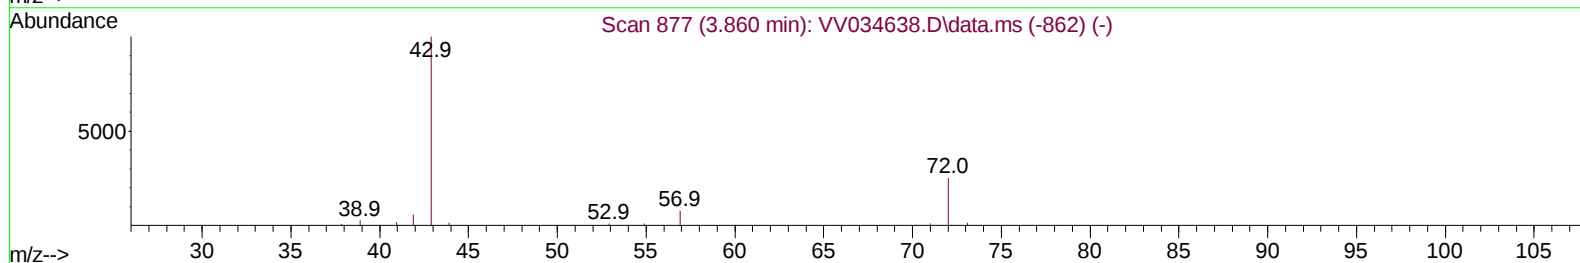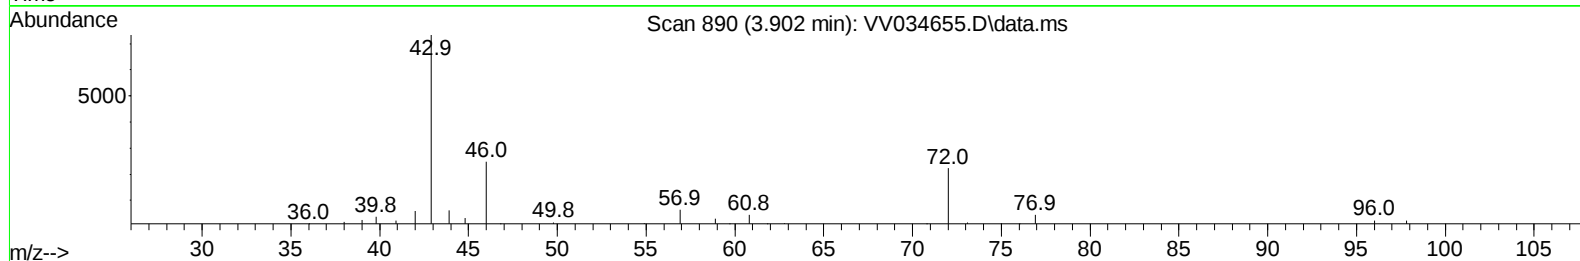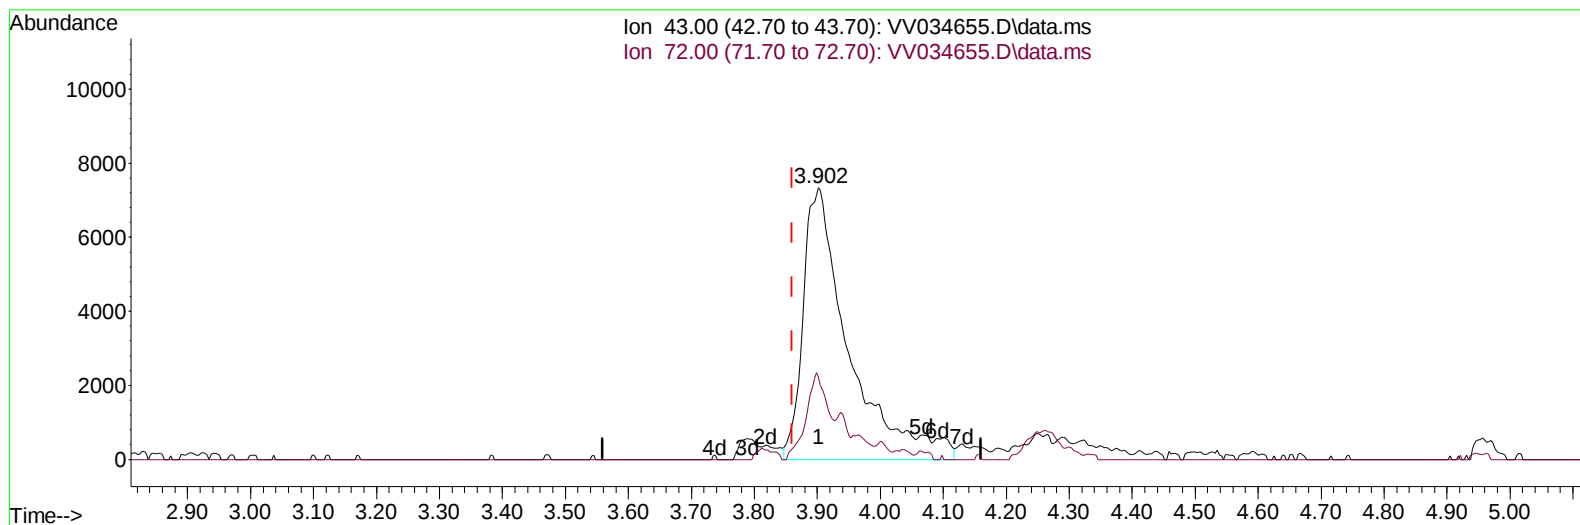

TIC: VV034655.D\data.ms

(22) 2-Butanone (T)

3.902min (+ 0.042) 15.73 ug/L m

response 36766

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	22.90	15.13
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034655.D
 Acq On : 15 Mar 2024 15:54
 Operator : SY/MD
 Sample : P1752-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL31

Manual IntegrationsAPPROVED

Quant Time: Mar 15 23:35:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 23:30:32 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/19/2024
 Supervised By :Semsettin Yesilyurt 03/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		339721	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		314079	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		145120	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		102617	34.844	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	69.680%	
7) Chloroethane-d5	1.532	69		91994	40.095	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	80.200%	
11) 1,1-Dichloroethene-d2	2.059	65		49770	37.368	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	74.740%	
21) 2-Butanone-d5	3.793	46		188883	95.906	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	95.910%	
24) Chloroform-d	4.249	84		214930	41.276	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	82.560%	
26) 1,2-Dichloroethane-d4	4.940	65		148184	43.549	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	87.100%	
32) Benzene-d6	4.960	84		410620	43.319	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	86.640%	
36) 1,2-Dichloropropane-d6	5.989	67		130045	44.955	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	89.900%	
41) Toluene-d8	7.243	98		351130	40.934	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	81.860%	
43) trans-1,3-Dichloroprop...	7.554	79		59015	40.625	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	81.260%	
47) 2-Hexanone-d5	8.024	63		129395	89.575	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	89.580%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84		182922	48.050	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	96.100%	
66) 1,2-Dichlorobenzene-d4	11.561	152		137178	46.246	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	92.500%	
Target Compounds							
						Qvalue	
12) 1,1-Dichloroethene	2.069	96		265396	104.330	ug/L #	81
13) Acetone	2.121	43		609984	257.638	ug/L	99
19) 1,1-Dichloroethane	3.111	63		63585	13.183	ug/L	98
20) cis-1,2-Dichloroethene	3.815	96		56837	21.276	ug/L	95
22) 2-Butanone	3.902	43		36766m	15.726	ug/L	
30) 1,1,1-Trichloroethane	4.513	97		29063	6.453	ug/L	99
34) Trichloroethene	5.837	95		17989	6.491	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034655.D
Acq On : 15 Mar 2024 15:54
Operator : SY/MD
Sample : P1752-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL31

Manual IntegrationsAPPROVED

Quant Time: Mar 15 23:35:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 23:30:32 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/19/2024
Supervised By :Semsettin Yesilyurt 03/19/2024

