

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034640.D
 Acq On : 15 Mar 2024 09:56
 Operator : SY/MD
 Sample : VV0315WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	178833	192676	14.35%	1.881%
2	1.526	144	151	169	rVB	156064	193670	14.43%	1.891%
3	2.056	306	316	340	rVB	322704	471178	35.10%	4.600%
4	2.449	431	438	447	rBV3	1649	2160	0.16%	0.021%
5	2.548	464	469	472	rBV3	1048	1195	0.09%	0.012%
6	2.600	482	485	488	rVB2	591	308	0.02%	0.003%
7	2.741	528	529	530	rBV	235	46	0.00%	0.000%
8	2.809	546	550	556	rBV2	330	387	0.03%	0.004%
9	2.899	574	578	579	rBV2	197	116	0.01%	0.001%
10	2.950	592	594	596	rVV2	205	88	0.01%	0.001%
11	2.995	606	608	611	rBV2	145	99	0.01%	0.001%
12	3.121	644	647	649	rBV	143	75	0.01%	0.001%
13	3.140	650	653	659	rVB3	367	366	0.03%	0.004%
14	3.169	659	662	665	rBV2	223	147	0.01%	0.001%
15	3.336	709	714	717	rBV2	224	204	0.02%	0.002%
16	3.387	728	730	731	rBV	197	66	0.00%	0.001%
17	3.455	746	751	758	rVB2	279	407	0.03%	0.004%
18	3.490	758	762	766	rBV2	283	286	0.02%	0.003%
19	3.558	780	783	787	rBV2	166	100	0.01%	0.001%
20	3.606	791	798	800	rBV2	180	205	0.02%	0.002%
21	3.690	820	824	828	rBV2	202	178	0.01%	0.002%
22	3.780	844	852	901	rBV	121435	326070	24.29%	3.184%
23	4.246	982	997	1026	rBV	214898	543868	40.52%	5.310%
24	4.564	1091	1096	1097	rBV2	327	271	0.02%	0.003%
25	4.654	1122	1124	1130	rBV2	345	316	0.02%	0.003%
26	4.722	1143	1145	1151	rVB3	181	108	0.01%	0.001%
27	4.895	1191	1199	1201	rBV2	355	543	0.04%	0.005%
28	4.953	1201	1217	1252	rBV2	506037	1342311	100.00%	13.106%
29	5.310	1324	1328	1329	rBV2	348	232	0.02%	0.002%
30	5.416	1356	1361	1362	rBV2	216	176	0.01%	0.002%
31	5.532	1386	1397	1423	rBV	393280	808285	60.22%	7.892%
32	5.834	1481	1491	1509	rVB5	7238	15220	1.13%	0.149%
33	5.989	1526	1539	1568	rBV	295288	609237	45.39%	5.948%
34	6.249	1619	1620	1625	rVB2	291	135	0.01%	0.001%
35	6.272	1625	1627	1628	rBV	256	145	0.01%	0.001%
36	6.310	1637	1639	1640	rBV	230	64	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034640.D
 Acq On : 15 Mar 2024 09:56
 Operator : SY/MD
 Sample : VV0315WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.358	1650	1654	1657	rBV2	283	180	0.01%	0.002%
38	6.394	1661	1665	1666	rBV	270	156	0.01%	0.002%
39	6.419	1671	1673	1676	rVB2	288	163	0.01%	0.002%
40	6.464	1683	1687	1688	rBV	289	133	0.01%	0.001%
41	6.590	1718	1726	1731	rBV4	1144	1762	0.13%	0.017%
42	6.773	1780	1783	1787	rVB	369	243	0.02%	0.002%
43	6.792	1787	1789	1791	rVB	316	126	0.01%	0.001%
44	6.847	1804	1806	1808	rVB	185	43	0.00%	0.000%
45	6.911	1816	1826	1855	rBV	150166	286742	21.36%	2.800%
46	7.117	1887	1890	1891	rBV2	405	196	0.01%	0.002%
47	7.136	1891	1896	1899	rBV4	1065	1240	0.09%	0.012%
48	7.243	1918	1929	1961	rBV	581403	1028420	76.62%	10.041%
49	7.554	2017	2026	2051	rBV2	101052	184450	13.74%	1.801%
50	7.709	2072	2074	2075	rBV	319	111	0.01%	0.001%
51	7.786	2096	2098	2100	rVB	337	135	0.01%	0.001%
52	7.805	2100	2104	2107	rBV2	346	336	0.03%	0.003%
53	7.853	2116	2119	2120	rBV	278	159	0.01%	0.002%
54	7.908	2133	2136	2138	rBV	190	119	0.01%	0.001%
55	7.989	2158	2161	2162	rBV2	188	85	0.01%	0.001%
56	8.021	2162	2171	2206	rBV	406611	746655	55.62%	7.290%
57	8.480	2310	2314	2316	rBV2	438	307	0.02%	0.003%
58	8.616	2354	2356	2358	rBV2	476	237	0.02%	0.002%
59	8.641	2361	2364	2368	rVB2	342	267	0.02%	0.003%
60	8.696	2379	2381	2387	rVB2	314	260	0.02%	0.003%
61	8.725	2387	2390	2392	rBV2	202	145	0.01%	0.001%
62	8.783	2397	2408	2437	rBV	593009	969619	72.24%	9.467%
63	9.085	2500	2502	2504	rVB2	355	143	0.01%	0.001%
64	9.140	2516	2519	2524	rBV3	374	305	0.02%	0.003%
65	9.397	2596	2599	2602	rBV2	236	187	0.01%	0.002%
66	9.451	2615	2616	2618	rVB	203	75	0.01%	0.001%
67	9.464	2618	2620	2624	rVB	252	132	0.01%	0.001%
68	9.487	2624	2627	2628	rBV	263	130	0.01%	0.001%
69	9.596	2658	2661	2665	rBV2	355	240	0.02%	0.002%
70	9.940	2764	2768	2770	rBV2	342	217	0.02%	0.002%
71	10.037	2796	2798	2801	rVB	215	118	0.01%	0.001%
72	10.066	2801	2807	2810	rBV2	217	292	0.02%	0.003%
73	10.152	2822	2834	2864	rBV	409023	650382	48.45%	6.350%
74	10.332	2888	2890	2891	rBV	156	69	0.01%	0.001%
75	10.349	2891	2895	2897	rVV2	324	229	0.02%	0.002%
76	10.577	2961	2966	2970	rBV2	204	198	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034640.D
 Acq On : 15 Mar 2024 09:56
 Operator : SY/MD
 Sample : VV0315WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.596	2970	2972	2973	rBV2	189	58	0.00%	0.001%
78	10.680	2996	2998	3002	rVB2	147	94	0.01%	0.001%
79	10.702	3002	3005	3008	rBV3	321	218	0.02%	0.002%
80	10.837	3044	3047	3049	rBV2	276	124	0.01%	0.001%
81	10.863	3051	3055	3057	rBV4	566	383	0.03%	0.004%
82	11.130	3134	3138	3142	rBV2	623	537	0.04%	0.005%
83	11.185	3144	3155	3185	rVV	584706	905490	67.46%	8.841%
84	11.471	3241	3244	3245	rBV	243	128	0.01%	0.001%
85	11.561	3259	3272	3295	rBV	585064	928276	69.16%	9.063%
86	11.869	3366	3368	3370	rBV	256	140	0.01%	0.001%
87	11.914	3380	3382	3384	rBV	233	116	0.01%	0.001%
88	12.091	3434	3437	3439	rBV2	290	169	0.01%	0.002%
89	12.384	3526	3528	3530	rVB2	529	137	0.01%	0.001%
90	12.448	3545	3548	3553	rBV2	425	360	0.03%	0.004%
91	12.554	3577	3581	3587	rBV2	354	384	0.03%	0.004%
92	12.702	3625	3627	3631	rBV	249	149	0.01%	0.001%
93	12.953	3703	3705	3709	rBV	297	166	0.01%	0.002%
94	13.210	3778	3785	3796	rVB7	1902	2642	0.20%	0.026%
95	13.390	3838	3841	3847	rBV2	487	447	0.03%	0.004%
96	13.448	3852	3859	3875	rVV2	8256	15120	1.13%	0.148%
97	13.609	3906	3909	3911	rBV	267	186	0.01%	0.002%
98	13.966	4018	4020	4024	rBV	324	194	0.01%	0.002%
99	14.069	4049	4052	4055	rBV	534	366	0.03%	0.004%
100	14.136	4071	4073	4074	rBV	296	112	0.01%	0.001%




Sum of corrected areas: 10241940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034640.D
Acq On : 15 Mar 2024 09:56
Operator : SY/MD
Sample : VV0315WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

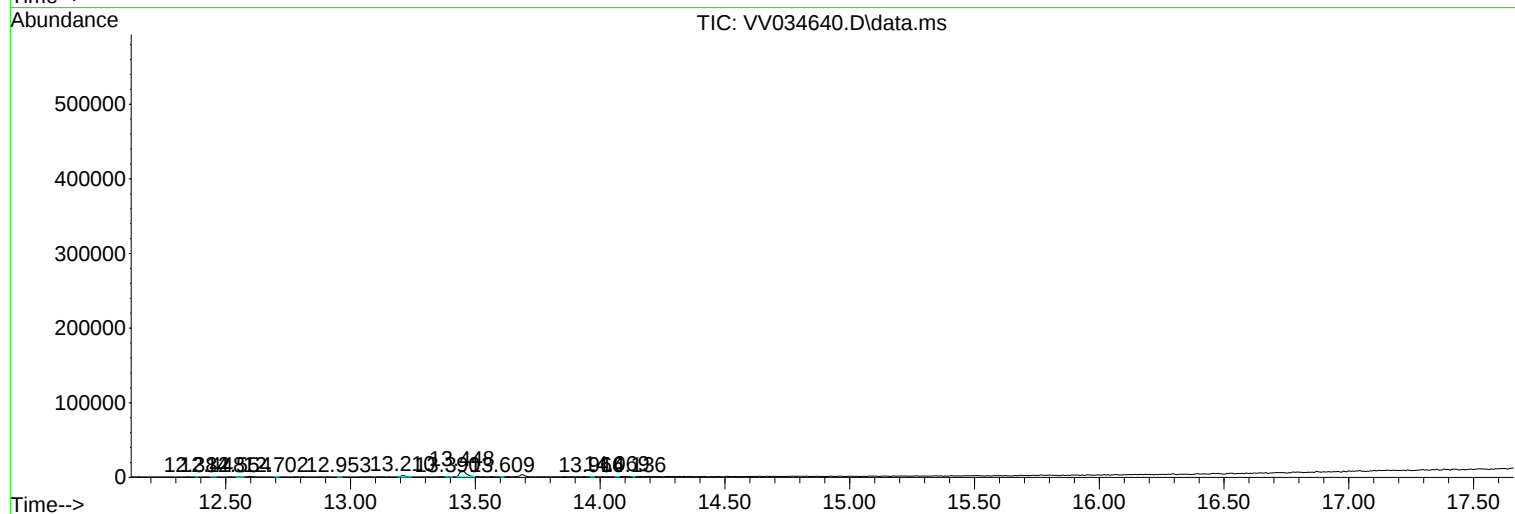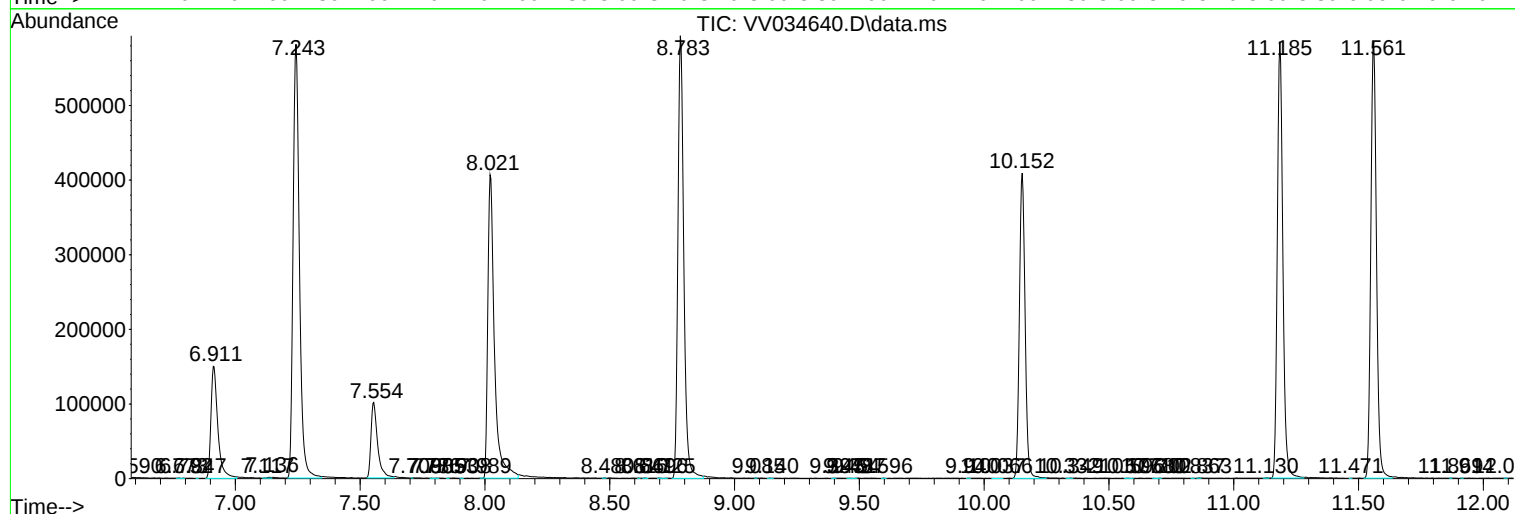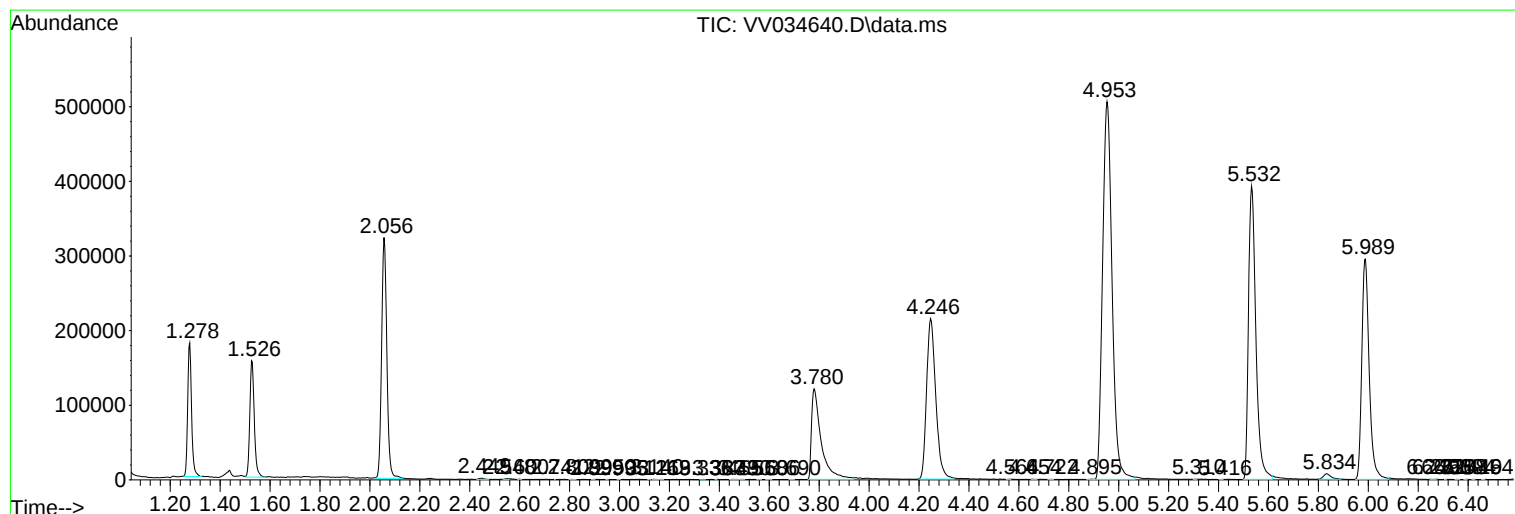

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034640.D
Acq On : 15 Mar 2024 09:56
Operator : SY/MD
Sample : VV0315WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034640.D
Acq On : 15 Mar 2024 09:56
Operator : SY/MD
Sample : VV0315WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc