

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034656.D
 Acq On : 15 Mar 2024 16:18
 Operator : SY/MD
 Sample : P1766-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	159934	164804	13.11%	1.582%
2	1.532	146	153	165	rVB	145281	163378	12.99%	1.568%
3	2.060	307	317	332	rBV2	303669	462483	36.78%	4.439%
4	2.712	517	520	523	rVB2	182	128	0.01%	0.001%
5	2.925	583	586	592	rVB2	386	338	0.03%	0.003%
6	2.963	592	598	602	rBV2	360	418	0.03%	0.004%
7	3.002	607	610	612	rBV	213	156	0.01%	0.001%
8	3.114	635	645	657	rVB	1126	2347	0.19%	0.023%
9	3.188	664	668	672	rVB2	175	136	0.01%	0.001%
10	3.211	672	675	677	rBV	160	108	0.01%	0.001%
11	3.391	728	731	733	rBV	233	192	0.02%	0.002%
12	3.439	743	746	748	rBV	219	146	0.01%	0.001%
13	3.510	765	768	771	rVB2	258	184	0.01%	0.002%
14	3.577	786	789	792	rBV2	178	111	0.01%	0.001%
15	3.606	793	798	804	rVB2	179	180	0.01%	0.002%
16	3.642	806	809	814	rVB2	228	186	0.01%	0.002%
17	3.670	814	818	821	rBV2	124	105	0.01%	0.001%
18	3.719	829	833	840	rVB2	220	273	0.02%	0.003%
19	3.796	848	857	893	rBV	115365	377782	30.04%	3.626%
20	4.249	983	998	1035	rBV	202236	514923	40.95%	4.943%
21	4.683	1130	1133	1137	rBV3	381	234	0.02%	0.002%
22	4.732	1145	1148	1152	rVB2	297	255	0.02%	0.002%
23	4.786	1162	1165	1170	rBV3	325	309	0.02%	0.003%
24	4.889	1191	1197	1201	rBV3	309	408	0.03%	0.004%
25	4.953	1201	1217	1255	rBV2	471468	1257537	100.00%	12.071%
26	5.262	1311	1313	1314	rBV	383	131	0.01%	0.001%
27	5.384	1348	1351	1354	rBV2	241	119	0.01%	0.001%
28	5.532	1387	1397	1434	rVV	361902	757393	60.23%	7.270%
29	5.831	1478	1490	1525	rBV	444958	903948	71.88%	8.677%
30	5.989	1527	1539	1572	rVB	274984	572851	45.55%	5.499%
31	6.246	1615	1619	1620	rBV	361	236	0.02%	0.002%
32	6.291	1631	1633	1638	rBV2	240	134	0.01%	0.001%
33	6.375	1656	1659	1660	rBV2	258	92	0.01%	0.001%
34	6.436	1672	1678	1680	rBV2	187	150	0.01%	0.001%
35	6.477	1687	1691	1693	rBV2	243	142	0.01%	0.001%
36	6.506	1697	1700	1704	rVB2	213	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034656.D
 Acq On : 15 Mar 2024 16:18
 Operator : SY/MD
 Sample : P1766-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.551	1710	1714	1717	rBV	209	139	0.01%	0.001%
38	6.577	1719	1722	1723	rBV	417	182	0.01%	0.002%
39	6.606	1723	1731	1735	rBV5	1035	1628	0.13%	0.016%
40	6.760	1777	1779	1784	rVB2	215	123	0.01%	0.001%
41	6.828	1795	1800	1803	rBV2	172	135	0.01%	0.001%
42	6.866	1810	1812	1816	rVB	215	141	0.01%	0.001%
43	6.915	1816	1827	1848	rBV	136210	260640	20.73%	2.502%
44	7.243	1918	1929	1963	rBV	518250	924670	73.53%	8.876%
45	7.555	2017	2026	2057	rBV	92119	171432	13.63%	1.646%
46	7.764	2088	2091	2092	rBV2	420	239	0.02%	0.002%
47	7.792	2097	2100	2102	rBV	444	262	0.02%	0.003%
48	7.860	2117	2121	2122	rBV2	360	179	0.01%	0.002%
49	7.918	2136	2139	2142	rBV2	180	105	0.01%	0.001%
50	7.963	2149	2153	2155	rBV2	184	138	0.01%	0.001%
51	8.024	2163	2172	2219	rVV	369933	725108	57.66%	6.960%
52	8.567	2339	2341	2347	rBV2	371	196	0.02%	0.002%
53	8.686	2372	2378	2381	rBV3	435	341	0.03%	0.003%
54	8.709	2382	2385	2388	rVB2	254	152	0.01%	0.001%
55	8.783	2398	2408	2440	rBV	523823	875258	69.60%	8.402%
56	8.985	2468	2471	2472	rBV	311	189	0.02%	0.002%
57	9.156	2522	2524	2525	rBV	257	103	0.01%	0.001%
58	9.300	2565	2569	2572	rVB2	118	103	0.01%	0.001%
59	9.323	2572	2576	2581	rBV	254	234	0.02%	0.002%
60	9.378	2589	2593	2597	rVB	367	225	0.02%	0.002%
61	9.400	2597	2600	2602	rBV2	153	99	0.01%	0.001%
62	9.471	2617	2622	2626	rBV3	190	208	0.02%	0.002%
63	9.590	2657	2659	2662	rBV	164	91	0.01%	0.001%
64	9.648	2674	2677	2684	rBV2	131	138	0.01%	0.001%
65	9.693	2689	2691	2695	rVV2	161	102	0.01%	0.001%
66	9.770	2712	2715	2720	rBV2	137	144	0.01%	0.001%
67	9.825	2726	2732	2736	rBV2	242	210	0.02%	0.002%
68	9.902	2755	2756	2760	rVB	326	101	0.01%	0.001%
69	10.005	2784	2788	2792	rBV2	170	180	0.01%	0.002%
70	10.153	2821	2834	2858	rBV	389702	610599	48.56%	5.861%
71	10.342	2891	2893	2896	rVB2	311	163	0.01%	0.002%
72	10.384	2901	2906	2909	rVB	206	203	0.02%	0.002%
73	10.410	2909	2914	2918	rBV	216	218	0.02%	0.002%
74	10.468	2929	2932	2936	rBV	135	96	0.01%	0.001%
75	10.522	2947	2949	2952	rVV2	324	215	0.02%	0.002%
76	10.554	2956	2959	2961	rBV2	176	122	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034656.D
 Acq On : 15 Mar 2024 16:18
 Operator : SY/MD
 Sample : P1766-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.792	3030	3033	3035	rVV	286	156	0.01%	0.001%
78	10.873	3055	3058	3061	rBV	192	139	0.01%	0.001%
79	11.005	3096	3099	3104	rVB	248	195	0.02%	0.002%
80	11.088	3123	3125	3128	rVB2	308	154	0.01%	0.001%
81	11.130	3135	3138	3144	rBV2	226	230	0.02%	0.002%
82	11.185	3144	3155	3183	rBV	512811	803867	63.92%	7.716%
83	11.406	3221	3224	3226	rVB2	369	183	0.01%	0.002%
84	11.468	3240	3243	3247	rVB	387	241	0.02%	0.002%
85	11.561	3258	3272	3293	rBV	536101	851929	67.75%	8.178%
86	11.808	3348	3349	3352	rBV	231	120	0.01%	0.001%
87	11.837	3356	3358	3360	rBV	199	95	0.01%	0.001%
88	12.297	3495	3501	3503	rBV	297	287	0.02%	0.003%
89	12.503	3559	3565	3567	rBV2	295	252	0.02%	0.002%
90	12.628	3600	3604	3607	rBV	245	193	0.02%	0.002%
91	12.725	3631	3634	3637	rBV	302	203	0.02%	0.002%
92	12.779	3649	3651	3654	rBV	189	116	0.01%	0.001%
93	12.847	3669	3672	3673	rBV	248	114	0.01%	0.001%
94	13.082	3742	3745	3749	rBV2	298	190	0.02%	0.002%
95	13.394	3838	3842	3848	rBV2	394	405	0.03%	0.004%
96	13.467	3861	3865	3868	rBV2	556	459	0.04%	0.004%
97	13.551	3888	3891	3896	rBV	299	294	0.02%	0.003%
98	13.763	3954	3957	3959	rBV2	339	210	0.02%	0.002%
99	13.779	3959	3962	3963	rBV	305	154	0.01%	0.001%
100	13.902	3997	4000	4001	rBV	238	137	0.01%	0.001%




Sum of corrected areas: 10417593

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034656.D
Acq On : 15 Mar 2024 16:18
Operator : SY/MD
Sample : P1766-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COGL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

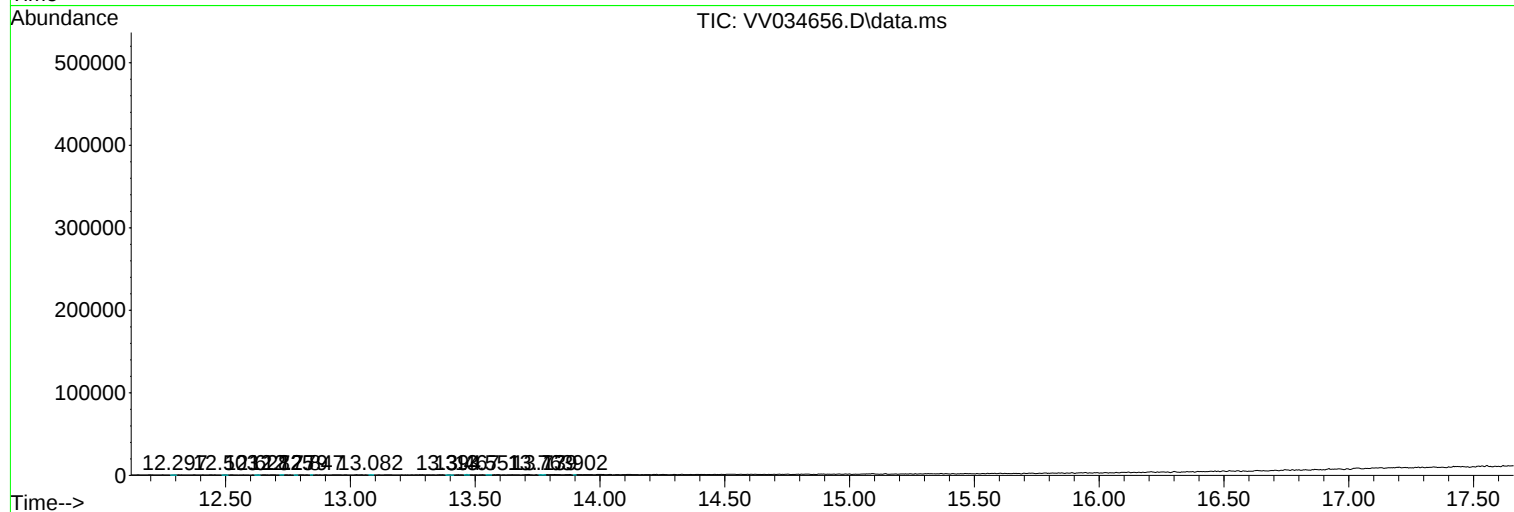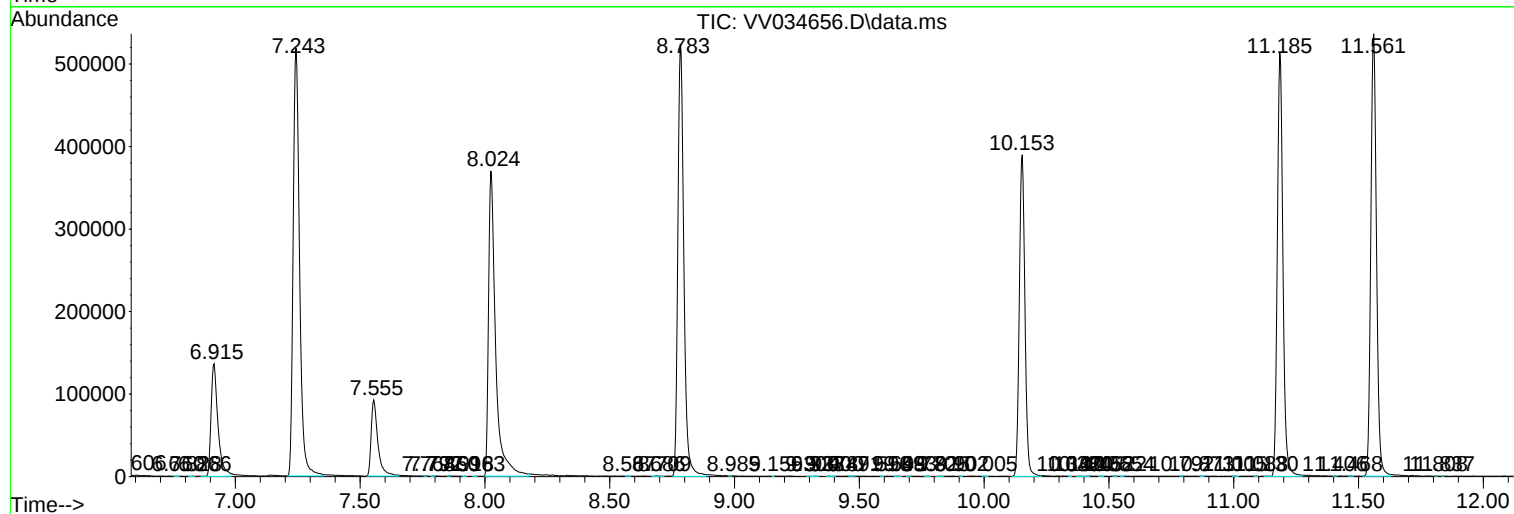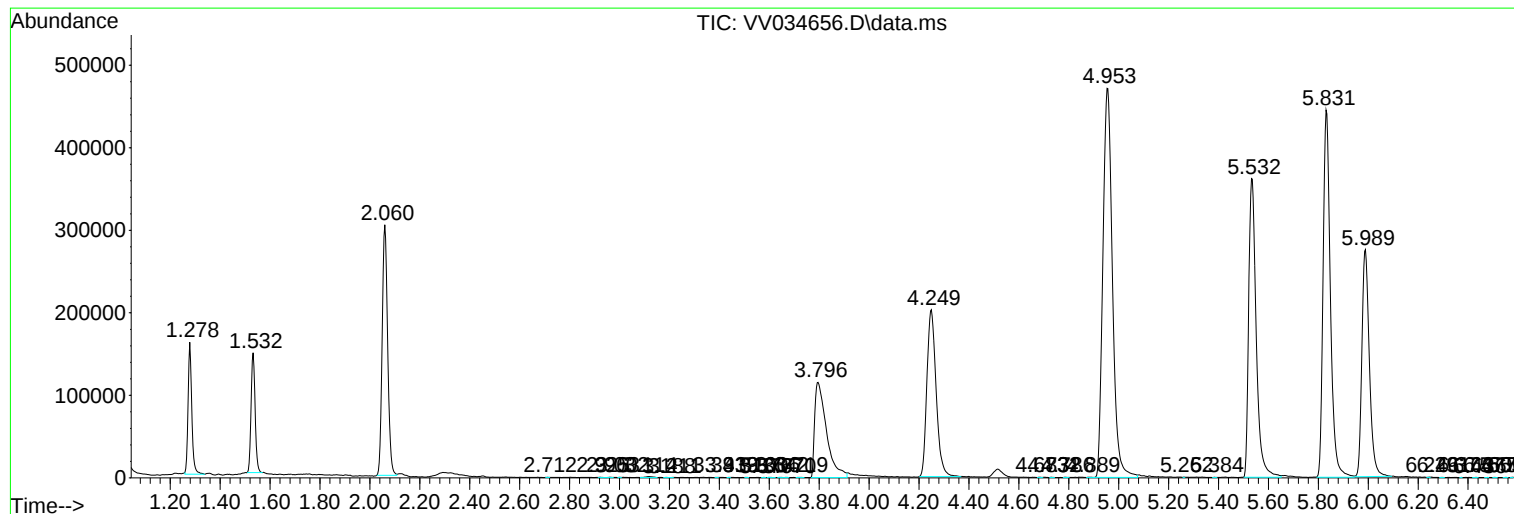

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034656.D
Acq On : 15 Mar 2024 16:18
Operator : SY/MD
Sample : P1766-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034656.D
Acq On : 15 Mar 2024 16:18
Operator : SY/MD
Sample : P1766-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
