

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034661.D
 Acq On : 15 Mar 2024 18:17
 Operator : SY/MD
 Sample : P1766-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	143120	152522	12.02%	1.504%
2	1.532	146	153	167	rBV	144483	166368	13.11%	1.641%
3	2.059	307	317	330	rBV	268030	390299	30.76%	3.850%
4	2.674	506	508	510	rVB2	276	111	0.01%	0.001%
5	2.822	550	554	559	rBV2	335	302	0.02%	0.003%
6	2.847	559	562	565	rBV2	353	199	0.02%	0.002%
7	2.886	571	574	581	rBV5	1054	1068	0.08%	0.011%
8	2.915	581	583	586	rVB2	444	202	0.02%	0.002%
9	3.082	632	635	637	rBV2	227	155	0.01%	0.002%
10	3.182	664	666	669	rVB2	202	106	0.01%	0.001%
11	3.201	669	672	677	rBV2	170	171	0.01%	0.002%
12	3.268	690	693	695	rBV	177	136	0.01%	0.001%
13	3.307	702	705	707	rBV	128	91	0.01%	0.001%
14	3.339	712	715	719	rBV2	112	114	0.01%	0.001%
15	3.391	729	731	735	rVB2	212	100	0.01%	0.001%
16	3.416	735	739	741	rBV	192	141	0.01%	0.001%
17	3.436	741	745	750	rVB2	272	263	0.02%	0.003%
18	3.471	750	756	760	rBV2	271	258	0.02%	0.003%
19	3.506	765	767	768	rBV	240	76	0.01%	0.001%
20	3.606	792	798	800	rBV2	217	173	0.01%	0.002%
21	3.793	845	856	897	rBV	111477	357925	28.21%	3.530%
22	4.246	982	997	1027	rBV	204708	529465	41.73%	5.222%
23	4.558	1091	1094	1095	rBV	405	218	0.02%	0.002%
24	4.728	1143	1147	1148	rBV2	371	252	0.02%	0.002%
25	4.770	1158	1160	1164	rBV	209	119	0.01%	0.001%
26	4.957	1202	1218	1258	rBV2	471699	1268664	100.00%	12.514%
27	5.378	1346	1349	1350	rBV	267	163	0.01%	0.002%
28	5.413	1357	1360	1362	rBV2	470	302	0.02%	0.003%
29	5.445	1367	1370	1374	rBV3	333	256	0.02%	0.003%
30	5.532	1386	1397	1436	rBV	424434	884122	69.69%	8.721%
31	5.831	1480	1490	1508	rBV2	11655	25914	2.04%	0.256%
32	5.989	1526	1539	1561	rBV	282917	585019	46.11%	5.770%
33	6.358	1652	1654	1661	rVB2	415	408	0.03%	0.004%
34	6.410	1669	1670	1674	rVB	174	85	0.01%	0.001%
35	6.442	1674	1680	1682	rBV2	226	205	0.02%	0.002%
36	6.477	1687	1691	1693	rBV2	151	115	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034661.D
 Acq On : 15 Mar 2024 18:17
 Operator : SY/MD
 Sample : P1766-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.503	1697	1699	1700	rBV	134	39	0.00%	0.000%
38	6.680	1750	1754	1755	rBV	334	195	0.02%	0.002%
39	6.815	1794	1796	1801	rVB	433	184	0.01%	0.002%
40	6.857	1807	1809	1814	rBB2	244	157	0.01%	0.002%
41	6.911	1814	1826	1856	rBV	139729	273411	21.55%	2.697%
42	7.243	1918	1929	1957	rBV	534598	947192	74.66%	9.343%
43	7.554	2016	2026	2051	rBV	94321	178635	14.08%	1.762%
44	7.828	2109	2111	2114	rBV2	418	240	0.02%	0.002%
45	7.908	2133	2136	2141	rVB2	204	130	0.01%	0.001%
46	7.940	2141	2146	2150	rBV3	310	309	0.02%	0.003%
47	7.976	2154	2157	2158	rBV	306	148	0.01%	0.001%
48	8.024	2163	2172	2213	rBV	402648	786582	62.00%	7.759%
49	8.580	2343	2345	2346	rBV	163	67	0.01%	0.001%
50	8.712	2384	2386	2387	rBV	175	64	0.01%	0.001%
51	8.783	2397	2408	2439	rBV	653158	1072928	84.57%	10.583%
52	9.117	2507	2512	2514	rBV3	483	463	0.04%	0.005%
53	9.146	2519	2521	2524	rVV	261	166	0.01%	0.002%
54	9.162	2524	2526	2531	rVB2	340	207	0.02%	0.002%
55	9.191	2533	2535	2539	rBV2	336	214	0.02%	0.002%
56	9.223	2543	2545	2548	rVB	273	113	0.01%	0.001%
57	9.246	2548	2552	2554	rBV	271	181	0.01%	0.002%
58	9.471	2617	2622	2626	rBV2	245	218	0.02%	0.002%
59	9.500	2630	2631	2632	rVB2	206	40	0.00%	0.000%
60	9.509	2632	2634	2635	rBV	303	124	0.01%	0.001%
61	9.564	2647	2651	2652	rBV	166	84	0.01%	0.001%
62	9.577	2653	2655	2656	rBV	168	58	0.00%	0.001%
63	9.622	2664	2669	2673	rVB2	290	253	0.02%	0.002%
64	9.667	2680	2683	2688	rVB	297	155	0.01%	0.002%
65	9.686	2688	2689	2690	rBV	210	65	0.01%	0.001%
66	9.728	2700	2702	2705	rBV	174	92	0.01%	0.001%
67	9.821	2728	2731	2733	rBV2	141	91	0.01%	0.001%
68	9.905	2753	2757	2759	rBV2	305	242	0.02%	0.002%
69	9.943	2766	2769	2774	rBV2	166	164	0.01%	0.002%
70	10.152	2822	2834	2857	rBV	402932	638149	50.30%	6.294%
71	10.320	2883	2886	2891	rBV2	679	565	0.04%	0.006%
72	10.406	2911	2913	2918	rVB	106	70	0.01%	0.001%
73	10.435	2918	2922	2926	rBV	176	181	0.01%	0.002%
74	10.551	2954	2958	2960	rBV	186	120	0.01%	0.001%
75	10.612	2975	2977	2981	rVB2	287	131	0.01%	0.001%
76	10.635	2981	2984	2987	rVB2	262	160	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034661.D
 Acq On : 15 Mar 2024 18:17
 Operator : SY/MD
 Sample : P1766-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.956	3082	3084	3088	rVB2	347	177	0.01%	0.002%
78	11.043	3109	3111	3114	rBV2	131	82	0.01%	0.001%
79	11.072	3117	3120	3126	rVB2	264	209	0.02%	0.002%
80	11.104	3128	3130	3133	rVB	249	109	0.01%	0.001%
81	11.123	3133	3136	3141	rBV2	363	276	0.02%	0.003%
82	11.185	3144	3155	3183	rBV	619913	971629	76.59%	9.584%
83	11.432	3230	3232	3234	rVB	283	102	0.01%	0.001%
84	11.458	3237	3240	3242	rBV3	386	279	0.02%	0.003%
85	11.561	3259	3272	3293	rBV	557877	893097	70.40%	8.809%
86	11.815	3350	3351	3353	rBV	220	92	0.01%	0.001%
87	11.857	3361	3364	3366	rBV	224	125	0.01%	0.001%
88	12.120	3443	3446	3448	rVB	398	202	0.02%	0.002%
89	12.136	3449	3451	3454	rBV2	290	185	0.01%	0.002%
90	12.320	3502	3508	3510	rBV2	347	286	0.02%	0.003%
91	12.400	3530	3533	3534	rBV	251	135	0.01%	0.001%
92	12.439	3542	3545	3548	rBV	235	140	0.01%	0.001%
93	12.844	3666	3671	3673	rBV3	449	337	0.03%	0.003%
94	13.178	3771	3775	3778	rBV2	397	353	0.03%	0.003%
95	13.320	3816	3819	3820	rBV	248	134	0.01%	0.001%
96	13.413	3846	3848	3850	rBV2	202	82	0.01%	0.001%
97	13.426	3850	3852	3857	rVV2	387	295	0.02%	0.003%
98	13.856	3984	3986	3990	rBV2	380	291	0.02%	0.003%
99	14.403	4151	4156	4159	rBV3	614	619	0.05%	0.006%
100	14.946	4323	4325	4329	rBV3	753	400	0.03%	0.004%




Sum of corrected areas: 10138310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034661.D
Acq On : 15 Mar 2024 18:17
Operator : SY/MD
Sample : P1766-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

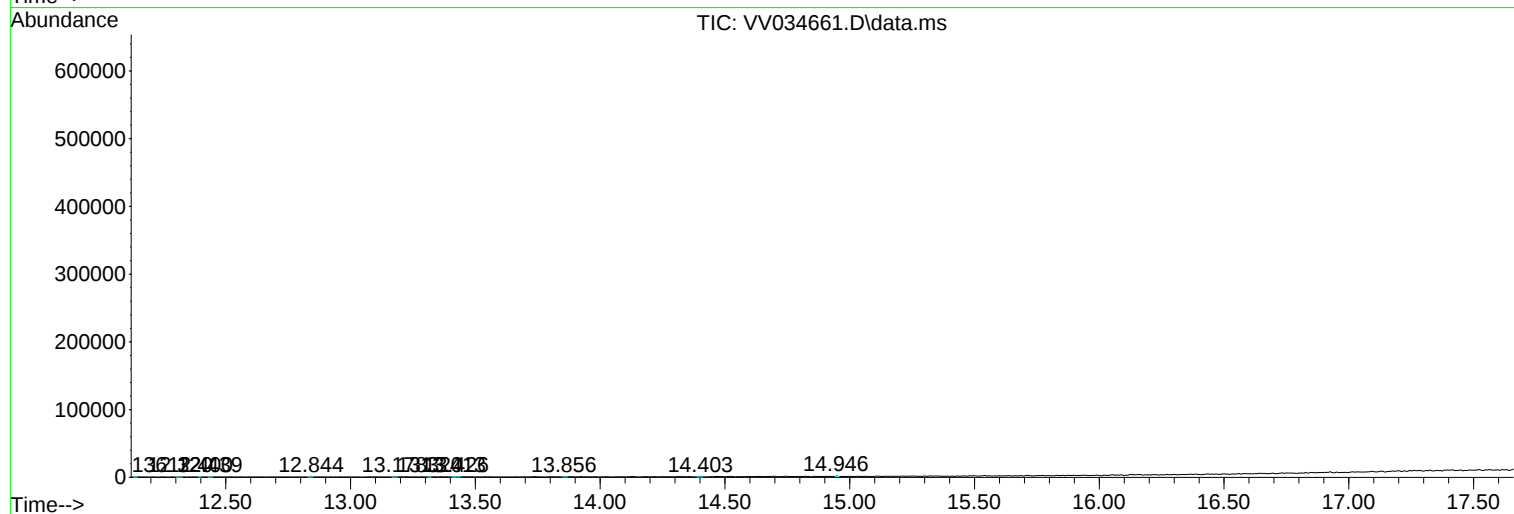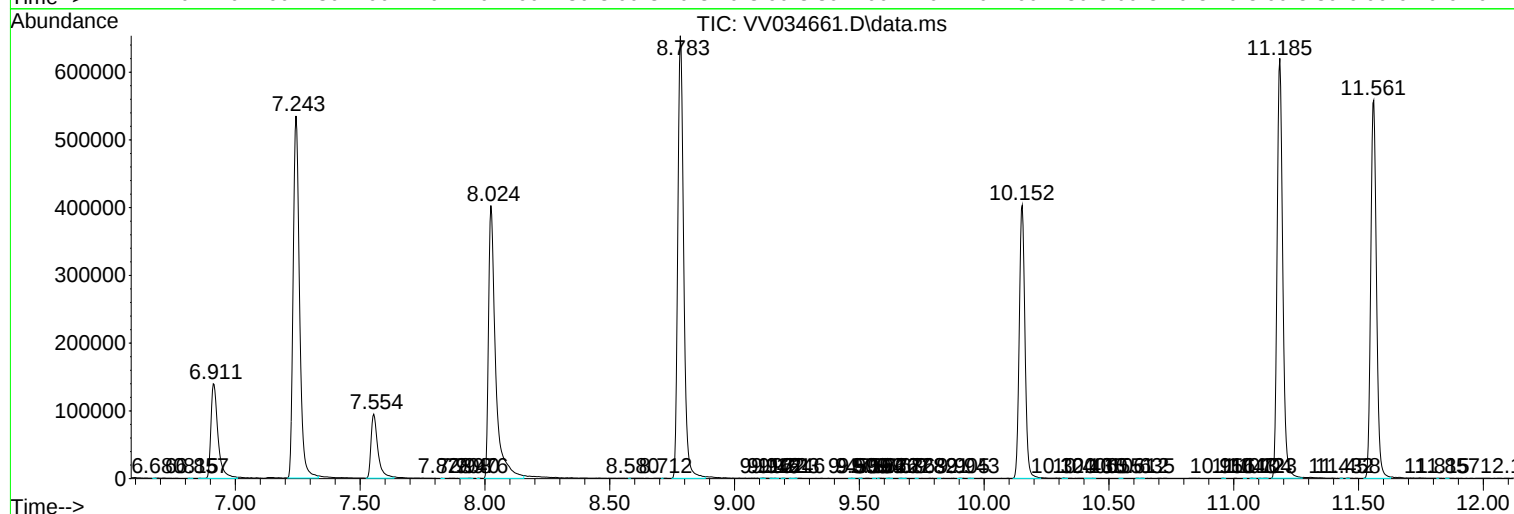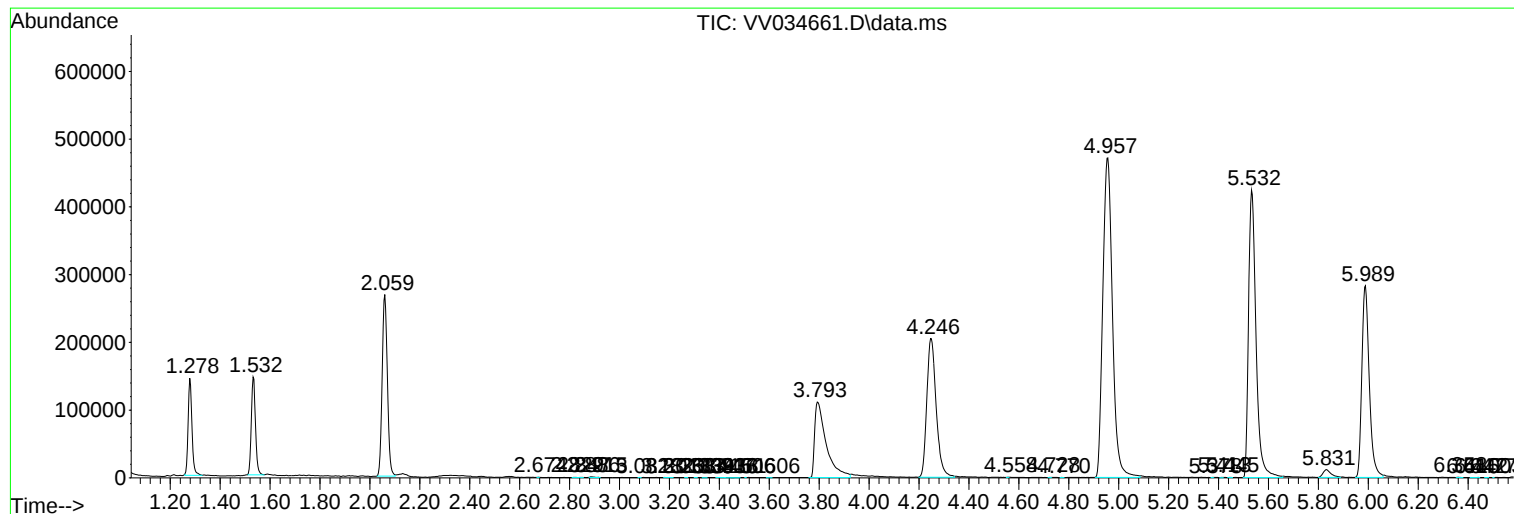

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034661.D
Acq On : 15 Mar 2024 18:17
Operator : SY/MD
Sample : P1766-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034661.D
Acq On : 15 Mar 2024 18:17
Operator : SY/MD
Sample : P1766-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
