

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034663.D
 Acq On : 15 Mar 2024 19:05
 Operator : SY/MD
 Sample : P1766-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	146554	155486	12.50%	1.606%
2	1.532	146	153	170	rVB	139792	165066	13.27%	1.705%
3	2.060	307	317	332	rBV	271502	392659	31.57%	4.055%
4	2.625	489	493	494	rBV	304	242	0.02%	0.002%
5	2.693	510	514	515	rBV	226	164	0.01%	0.002%
6	2.812	549	551	558	rVB2	267	225	0.02%	0.002%
7	2.963	596	598	600	rBV	310	126	0.01%	0.001%
8	3.037	620	621	622	rBV	264	73	0.01%	0.001%
9	3.076	630	633	635	rBV	127	62	0.00%	0.001%
10	3.133	650	651	652	rVB	121	23	0.00%	0.000%
11	3.169	658	662	666	rBV2	173	179	0.01%	0.002%
12	3.191	667	669	671	rBV	192	99	0.01%	0.001%
13	3.275	692	695	697	rBV2	177	128	0.01%	0.001%
14	3.301	701	703	704	rBV	119	50	0.00%	0.001%
15	3.317	704	708	709	rBV	202	123	0.01%	0.001%
16	3.404	732	735	736	rBV	119	68	0.01%	0.001%
17	3.494	759	763	764	rBV2	126	83	0.01%	0.001%
18	3.529	772	774	779	rVB2	253	129	0.01%	0.001%
19	3.555	779	782	784	rBV	144	69	0.01%	0.001%
20	3.564	784	785	786	rBV	145	31	0.00%	0.000%
21	3.606	794	798	800	rBV2	89	73	0.01%	0.001%
22	3.619	800	802	805	rVB2	96	45	0.00%	0.000%
23	3.632	805	806	808	rBV	157	58	0.00%	0.001%
24	3.757	841	845	848	rBV	262	220	0.02%	0.002%
25	3.796	848	857	898	rBV	102806	319217	25.67%	3.297%
26	4.249	981	998	1029	rBV	198580	511732	41.15%	5.285%
27	4.632	1115	1117	1120	rVB2	336	193	0.02%	0.002%
28	4.651	1120	1123	1126	rBV2	371	317	0.03%	0.003%
29	4.674	1127	1130	1133	rVB3	380	256	0.02%	0.003%
30	4.696	1133	1137	1140	rBV2	356	271	0.02%	0.003%
31	4.773	1156	1161	1164	rBV2	217	198	0.02%	0.002%
32	4.844	1180	1183	1185	rBV2	234	192	0.02%	0.002%
33	4.879	1191	1194	1195	rBV	334	200	0.02%	0.002%
34	4.957	1201	1218	1251	rBV2	470083	1243654	100.00%	12.844%
35	5.275	1314	1317	1318	rBV2	330	184	0.01%	0.002%
36	5.375	1346	1348	1352	rVB2	358	219	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034663.D
 Acq On : 15 Mar 2024 19:05
 Operator : SY/MD
 Sample : P1766-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.397	1352	1355	1358	rBV	103	88	0.01%	0.001%
38	5.416	1358	1361	1364	rVV2	181	130	0.01%	0.001%
39	5.458	1370	1374	1376	rBV2	306	229	0.02%	0.002%
40	5.532	1384	1397	1433	rBV	410039	848268	68.21%	8.761%
41	5.838	1482	1492	1507	rVB3	6854	14418	1.16%	0.149%
42	5.989	1525	1539	1569	rBV	266301	553547	44.51%	5.717%
43	6.243	1616	1618	1619	rBV	278	137	0.01%	0.001%
44	6.313	1638	1640	1643	rVB	473	197	0.02%	0.002%
45	6.333	1643	1646	1648	rBV	151	93	0.01%	0.001%
46	6.346	1648	1650	1653	rVV	267	149	0.01%	0.002%
47	6.387	1660	1663	1664	rBV	124	78	0.01%	0.001%
48	6.436	1673	1678	1679	rBV2	225	177	0.01%	0.002%
49	6.468	1685	1688	1690	rBV2	63	29	0.00%	0.000%
50	6.484	1690	1693	1694	rBV	156	54	0.00%	0.001%
51	6.583	1719	1724	1726	rBV3	641	661	0.05%	0.007%
52	6.702	1755	1761	1763	rBV3	466	439	0.04%	0.005%
53	6.747	1773	1775	1776	rBV2	171	93	0.01%	0.001%
54	6.870	1811	1813	1814	rBV	136	64	0.01%	0.001%
55	6.876	1814	1815	1816	rVB	244	47	0.00%	0.000%
56	6.915	1816	1827	1858	rBV	129135	254859	20.49%	2.632%
57	7.243	1918	1929	1958	rBV	509246	909882	73.16%	9.397%
58	7.555	2017	2026	2055	rBV2	91607	169679	13.64%	1.752%
59	7.821	2107	2109	2116	rVB3	458	330	0.03%	0.003%
60	7.915	2133	2138	2142	rBV	238	220	0.02%	0.002%
61	7.992	2159	2162	2163	rBV2	292	144	0.01%	0.001%
62	8.024	2163	2172	2223	rVV	368500	736240	59.20%	7.604%
63	8.474	2310	2312	2314	rVB2	371	159	0.01%	0.002%
64	8.506	2318	2322	2326	rBV2	529	545	0.04%	0.006%
65	8.567	2340	2341	2342	rBV	182	44	0.00%	0.000%
66	8.616	2353	2356	2360	rBV3	238	260	0.02%	0.003%
67	8.664	2368	2371	2372	rBV2	437	238	0.02%	0.002%
68	8.783	2398	2408	2447	rBV	609717	1016329	81.72%	10.496%
69	9.050	2489	2491	2492	rBV2	166	89	0.01%	0.001%
70	9.063	2492	2495	2498	rVB	429	287	0.02%	0.003%
71	9.153	2520	2523	2525	rBV2	259	160	0.01%	0.002%
72	9.201	2537	2538	2539	rBV2	292	91	0.01%	0.001%
73	9.300	2565	2569	2572	rBV	119	87	0.01%	0.001%
74	9.329	2573	2578	2579	rBV2	270	179	0.01%	0.002%
75	9.371	2589	2591	2594	rBV	138	72	0.01%	0.001%
76	9.770	2714	2715	2716	rVB	166	32	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034663.D
 Acq On : 15 Mar 2024 19:05
 Operator : SY/MD
 Sample : P1766-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.789	2716	2721	2723	rBV	141	133	0.01%	0.001%
78	9.860	2741	2743	2744	rBV	153	48	0.00%	0.000%
79	9.921	2758	2762	2764	rBV2	157	126	0.01%	0.001%
80	9.947	2769	2770	2773	rVB	270	83	0.01%	0.001%
81	10.152	2822	2834	2857	rBV	387031	607575	48.85%	6.275%
82	10.464	2927	2931	2935	rBV2	302	287	0.02%	0.003%
83	10.538	2952	2954	2960	rVB2	223	177	0.01%	0.002%
84	10.898	3062	3066	3071	rBV2	294	245	0.02%	0.003%
85	10.924	3071	3074	3076	rBV	182	141	0.01%	0.001%
86	11.050	3110	3113	3116	rBV	276	190	0.02%	0.002%
87	11.185	3144	3155	3180	rBV	592634	923987	74.30%	9.543%
88	11.484	3246	3248	3250	rBV	211	109	0.01%	0.001%
89	11.561	3260	3272	3302	rBV	532273	846957	68.10%	8.747%
90	11.818	3349	3352	3354	rBV2	421	211	0.02%	0.002%
91	11.863	3363	3366	3369	rVB2	295	170	0.01%	0.002%
92	12.040	3415	3421	3424	rBV	266	278	0.02%	0.003%
93	12.342	3513	3515	3517	rBV	235	76	0.01%	0.001%
94	12.435	3542	3544	3545	rBV	177	49	0.00%	0.001%
95	12.619	3599	3601	3602	rBV	232	96	0.01%	0.001%
96	12.728	3632	3635	3637	rBV	282	205	0.02%	0.002%
97	13.168	3770	3772	3774	rBV3	206	103	0.01%	0.001%
98	13.213	3780	3786	3789	rBV2	330	363	0.03%	0.004%
99	13.503	3874	3876	3880	rVB2	347	141	0.01%	0.001%


Sum of corrected areas: 9682688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034663.D
Acq On : 15 Mar 2024 19:05
Operator : SY/MD
Sample : P1766-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

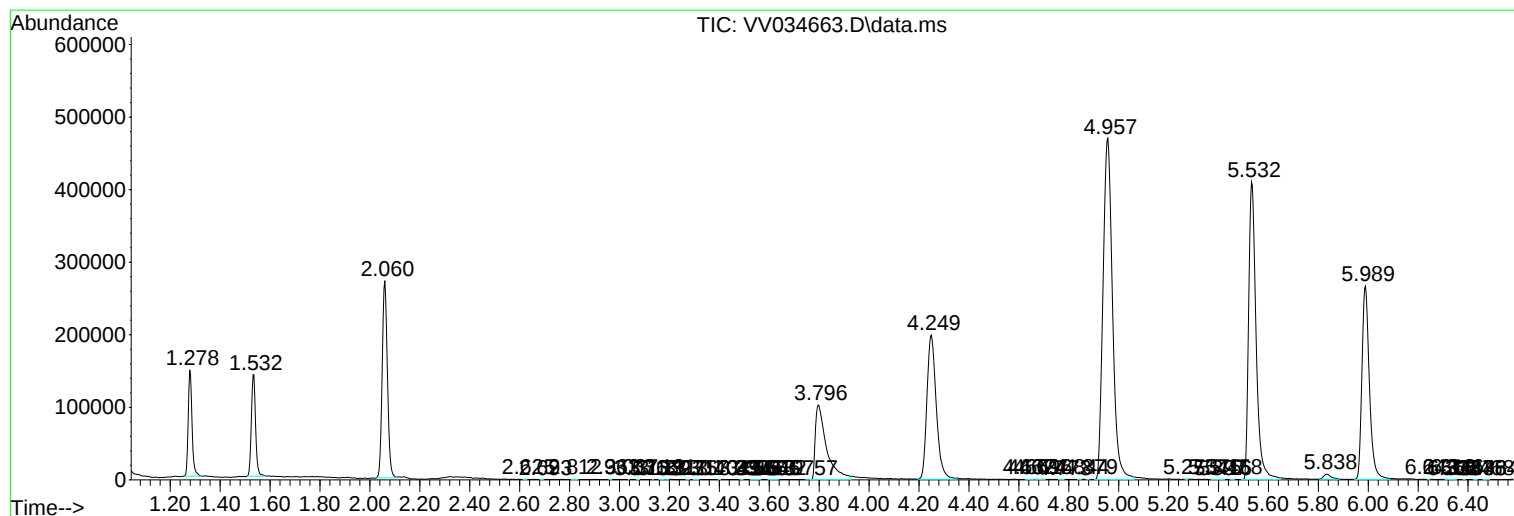

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034663.D
Acq On : 15 Mar 2024 19:05
Operator : SY/MD
Sample : P1766-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034663.D
Acq On : 15 Mar 2024 19:05
Operator : SY/MD
Sample : P1766-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc