

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034665.D
 Acq On : 15 Mar 2024 20:17
 Operator : SY/MD
 Sample : VV0315WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	161656	169980	12.89%	1.676%
2	1.532	146	153	164	rBV	154046	175726	13.32%	1.733%
3	2.060	306	317	335	rBV	295530	433953	32.90%	4.279%
4	2.346	403	406	411	rBV2	365	350	0.03%	0.003%
5	2.539	463	466	467	rBV	166	106	0.01%	0.001%
6	2.565	471	474	479	rVV2	197	180	0.01%	0.002%
7	2.703	511	517	518	rBV3	810	675	0.05%	0.007%
8	2.970	596	600	605	rBV2	151	178	0.01%	0.002%
9	2.999	605	609	613	rVV2	255	228	0.02%	0.002%
10	3.073	629	632	636	rVB2	199	134	0.01%	0.001%
11	3.102	638	641	644	rBV2	358	229	0.02%	0.002%
12	3.201	669	672	674	rBV2	258	113	0.01%	0.001%
13	3.349	715	718	720	rBV	161	89	0.01%	0.001%
14	3.439	739	746	748	rBV	307	356	0.03%	0.004%
15	3.677	816	820	823	rBV	146	105	0.01%	0.001%
16	3.696	823	826	829	rBV2	97	92	0.01%	0.001%
17	3.754	841	844	847	rBV2	177	99	0.01%	0.001%
18	3.796	848	857	892	rBV2	105439	321549	24.38%	3.170%
19	4.246	982	997	1030	rBV2	208576	541218	41.03%	5.336%
20	4.574	1096	1099	1103	rBV4	742	682	0.05%	0.007%
21	4.658	1121	1125	1132	rBV2	196	231	0.02%	0.002%
22	4.725	1142	1146	1149	rBV3	519	498	0.04%	0.005%
23	4.954	1201	1217	1246	rBV2	492722	1319047	100.00%	13.005%
24	5.468	1374	1377	1380	rBV2	257	197	0.01%	0.002%
25	5.532	1386	1397	1426	rBV	414800	858169	65.06%	8.461%
26	5.835	1481	1491	1511	rVB5	9666	22211	1.68%	0.219%
27	5.912	1513	1515	1518	rVB2	304	121	0.01%	0.001%
28	5.928	1518	1520	1522	rBV2	185	104	0.01%	0.001%
29	5.944	1523	1525	1526	rBV	229	81	0.01%	0.001%
30	5.989	1526	1539	1567	rBV	280602	586351	44.45%	5.781%
31	6.191	1599	1602	1604	rBV3	445	289	0.02%	0.003%
32	6.233	1612	1615	1616	rBV	294	117	0.01%	0.001%
33	6.285	1628	1631	1635	rVB3	362	220	0.02%	0.002%
34	6.307	1635	1638	1642	rVB2	128	99	0.01%	0.001%
35	6.333	1642	1646	1649	rBV2	193	156	0.01%	0.002%
36	6.352	1650	1652	1655	rBV	212	121	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034665.D
 Acq On : 15 Mar 2024 20:17
 Operator : SY/MD
 Sample : VV0315WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.420	1671	1673	1677	rBV	121	103	0.01%	0.001%
38	6.526	1700	1706	1708	rBV2	152	168	0.01%	0.002%
39	6.593	1719	1727	1728	rBV4	1080	1226	0.09%	0.012%
40	6.789	1786	1788	1794	rVB2	363	216	0.02%	0.002%
41	6.822	1795	1798	1800	rBV2	235	126	0.01%	0.001%
42	6.870	1811	1813	1816	rBV2	166	98	0.01%	0.001%
43	6.915	1816	1827	1854	rBV	137047	266966	20.24%	2.632%
44	7.243	1917	1929	1964	rBV	549465	982145	74.46%	9.683%
45	7.555	2017	2026	2059	rBV	93598	180077	13.65%	1.775%
46	7.857	2118	2120	2122	rBV2	256	97	0.01%	0.001%
47	7.908	2130	2136	2137	rBV	604	418	0.03%	0.004%
48	7.953	2147	2150	2152	rBV2	170	105	0.01%	0.001%
49	7.973	2154	2156	2159	rVB3	270	163	0.01%	0.002%
50	8.024	2163	2172	2214	rBV	378332	757923	57.46%	7.473%
51	8.513	2320	2324	2328	rBV3	302	362	0.03%	0.004%
52	8.571	2338	2342	2345	rBV2	204	204	0.02%	0.002%
53	8.683	2375	2377	2383	rVB	248	177	0.01%	0.002%
54	8.715	2385	2387	2389	rBV	363	118	0.01%	0.001%
55	8.783	2397	2408	2441	rBV	598736	1007194	76.36%	9.930%
56	9.214	2540	2542	2546	rVB2	201	89	0.01%	0.001%
57	9.236	2547	2549	2552	rBV	281	159	0.01%	0.002%
58	9.278	2559	2562	2566	rBV	101	90	0.01%	0.001%
59	9.301	2566	2569	2570	rBV	225	115	0.01%	0.001%
60	9.423	2604	2607	2614	rBV2	143	164	0.01%	0.002%
61	9.474	2619	2623	2624	rBV	411	258	0.02%	0.003%
62	9.522	2635	2638	2639	rBV2	443	238	0.02%	0.002%
63	9.648	2674	2677	2681	rBV	124	116	0.01%	0.001%
64	9.735	2701	2704	2707	rBV	231	221	0.02%	0.002%
65	9.809	2724	2727	2731	rBV2	221	164	0.01%	0.002%
66	9.876	2745	2748	2751	rBV3	735	419	0.03%	0.004%
67	9.934	2763	2766	2768	rBV	200	132	0.01%	0.001%
68	10.098	2814	2817	2822	rVB2	223	159	0.01%	0.002%
69	10.153	2822	2834	2854	rBV	395680	633416	48.02%	6.245%
70	10.336	2889	2891	2894	rVB2	393	230	0.02%	0.002%
71	10.371	2897	2902	2905	rBV	398	338	0.03%	0.003%
72	10.481	2929	2936	2947	rVB3	811	1341	0.10%	0.013%
73	10.539	2952	2954	2955	rBV	175	76	0.01%	0.001%
74	10.677	2994	2997	2999	rBV	241	174	0.01%	0.002%
75	10.776	3024	3028	3031	rBV2	153	128	0.01%	0.001%
76	10.805	3035	3037	3042	rVB2	403	254	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
 Data File : VV034665.D
 Acq On : 15 Mar 2024 20:17
 Operator : SY/MD
 Sample : VV0315WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

77	10.831	3042	3045	3049	rBV2	308	317	0.02%	0.003%
78	10.863	3050	3055	3062	rVB3	860	1305	0.10%	0.013%
79	10.924	3071	3074	3078	rBV	253	157	0.01%	0.002%
80	10.976	3088	3090	3092	rBV2	250	142	0.01%	0.001%
81	11.005	3097	3099	3101	rBV2	157	93	0.01%	0.001%
82	11.111	3129	3132	3134	rBV2	503	328	0.02%	0.003%
83	11.124	3134	3136	3137	rBV2	687	342	0.03%	0.003%
84	11.185	3144	3155	3184	rBV	593048	932287	70.68%	9.192%
85	11.407	3220	3224	3228	rVB3	447	435	0.03%	0.004%
86	11.484	3246	3248	3249	rBV3	244	98	0.01%	0.001%
87	11.500	3250	3253	3257	rVB3	420	289	0.02%	0.003%
88	11.561	3257	3272	3297	rBV	554610	905419	68.64%	8.927%
89	11.751	3329	3331	3334	rVB	371	171	0.01%	0.002%
90	12.503	3562	3565	3567	rBV2	164	120	0.01%	0.001%
91	12.587	3588	3591	3597	rBV5	1016	1042	0.08%	0.010%
92	12.654	3609	3612	3613	rBV	130	81	0.01%	0.001%
93	12.709	3626	3629	3633	rVB2	347	230	0.02%	0.002%
94	12.828	3664	3666	3669	rBV2	289	167	0.01%	0.002%
95	13.001	3717	3720	3722	rBV2	310	194	0.01%	0.002%
96	13.210	3775	3785	3794	rBV5	2906	4545	0.34%	0.045%
97	13.268	3801	3803	3806	rBV2	296	101	0.01%	0.001%
98	13.448	3850	3859	3872	rBV	10886	18010	1.37%	0.178%
99	13.612	3908	3910	3914	rVB2	336	129	0.01%	0.001%
100	13.683	3925	3932	3942	rBV2	4007	6322	0.48%	0.062%




Sum of corrected areas: 10142545

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034665.D
Acq On : 15 Mar 2024 20:17
Operator : SY/MD
Sample : VV0315WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

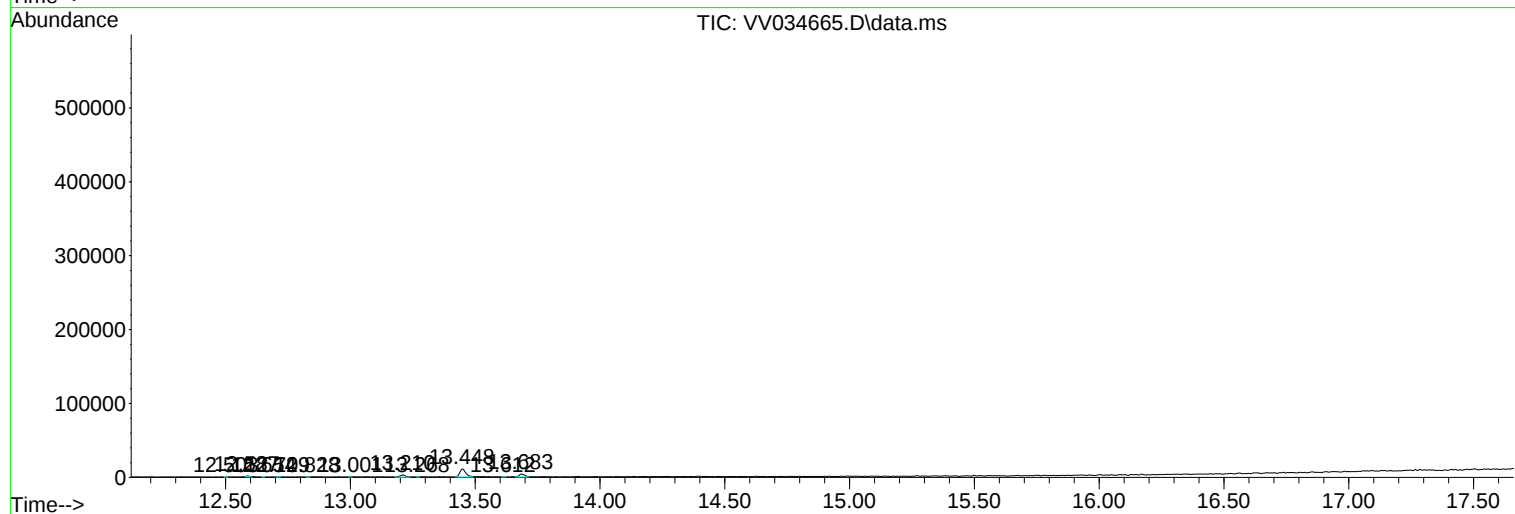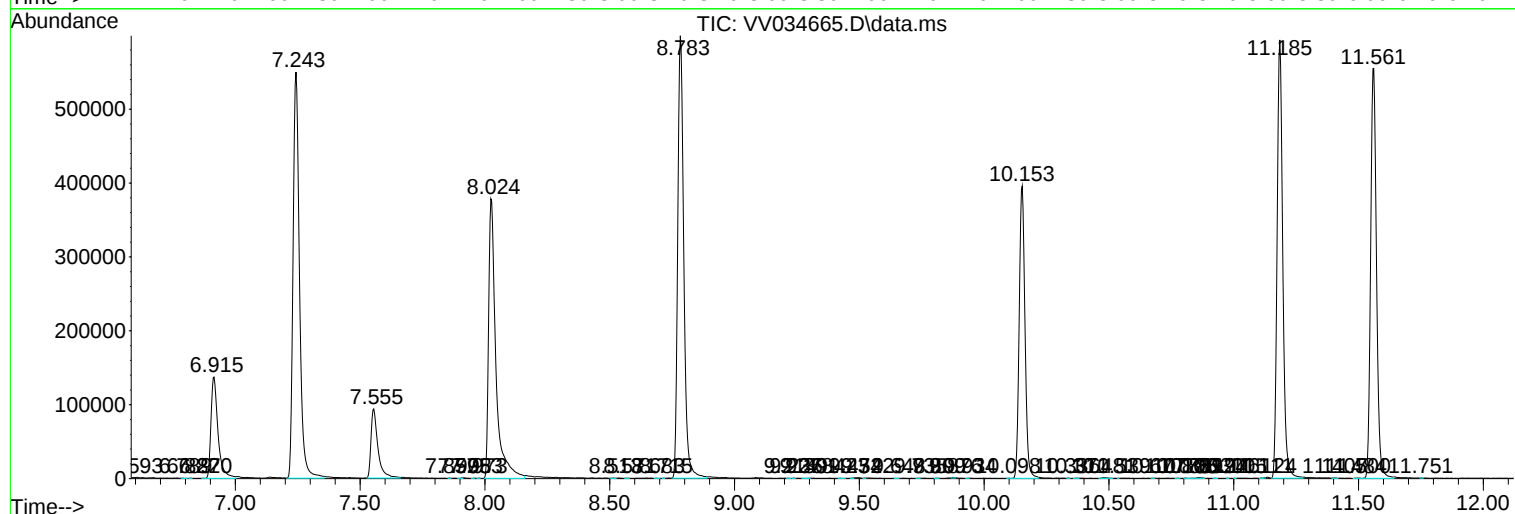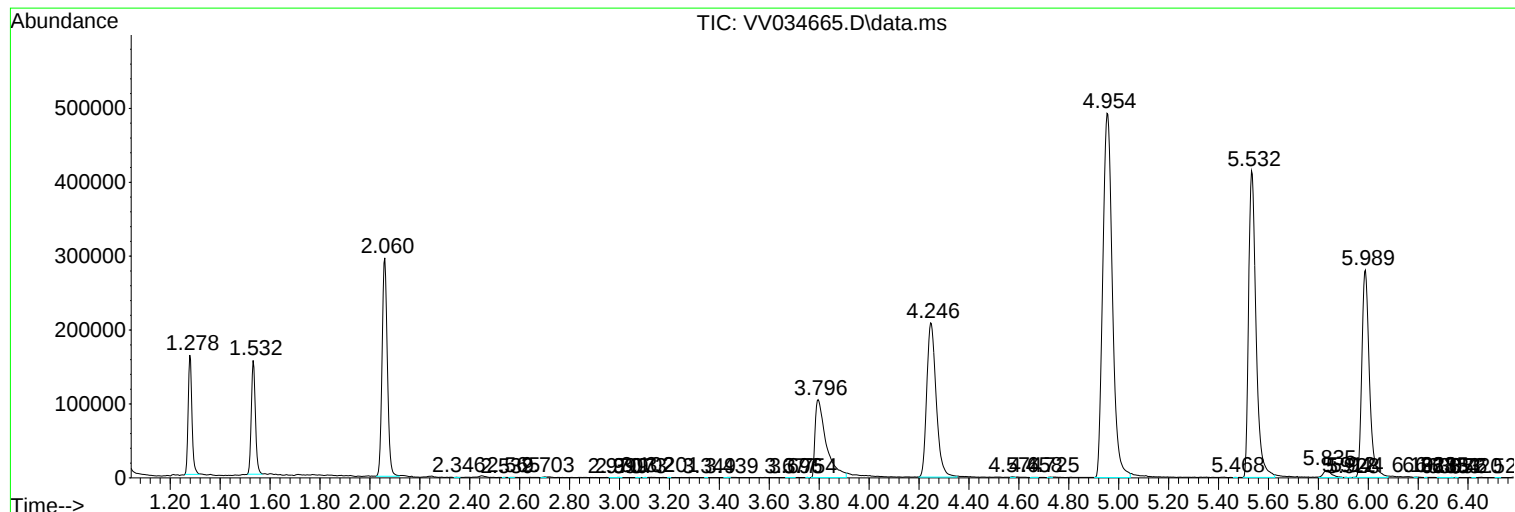

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034665.D
Acq On : 15 Mar 2024 20:17
Operator : SY/MD
Sample : VV0315WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031524\
Data File : VV034665.D
Acq On : 15 Mar 2024 20:17
Operator : SY/MD
Sample : VV0315WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc